



Standard Test Method for Spontaneous Heating Values of Liquids and Solids (Differential Mackey Test)¹

This standard is issued under the fixed designation D3523; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the non-adiabatic determination of the spontaneous heating values (SHV) of liquids and solids. It is applicable to substances that are not completely volatile at the test temperature. Spontaneous heating values obtained by this test method are qualitative indications of the degree of self-heating that may be expected to occur upon exposure of the sample to air at the test temperature.

1.2 Values obtained by this method are applicable to liquids and solids supported on cellulosic surfaces. They are not applicable to liquids on metal surfaces, on contaminated surfaces, or at pressures above atmospheric.

1.3 Spontaneous heating values determined by the present test method are regarded only as qualitative measurements of self-heating which occurs under the conditions of the test. The test method does not purport to produce a quantitative measure of the enthalpy of reaction of the sample with air at a given test temperature. Such data can be obtained by the use of an adiabatic calorimeter. The existence, under the test conditions, of a positive temperature difference between the sample and the reference is evidence of a thermochemical reaction in the sample.

1.4 The magnitude of the measured temperature difference is a semiquantitative indication of the enthalpy and rate of that reaction. Since factors such as heat loss from the sample to the bath and quenching of the reaction due to too rapid consumption of oxygen affect the amount and duration of the measured heat effect, care must be taken not to attribute too much quantitative significance to the test results. It is sufficient, for the purpose of this test, to determine whether or not the sample is capable of undergoing a self-heating reaction of sufficient magnitude and rapidity to produce a detectable thermal effect. The spontaneous heating value (SHV) can be lower than the test temperature. A negative result does not preclude spontaneous heating initiating at a temperature higher than the test temperature.

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee D02.11 on Engineering Sciences of High Performance Fluids and Solids.

Current edition approved May 1, 2007. Published June 2007. Originally approved in 1976. Last previous edition approved in 2002 as D3523 – 92 (2002). DOI: 10.1520/D3523-92R07.

1.5 This standard should be used to measure and describe the response of materials, products, or assemblies to heat and flame under controlled conditions and should not be used to describe or appraise the fire-hazard or fire-risk of materials, products, or assemblies under actual fire conditions. However, results of this test may be used as elements of a fire-hazard assessment or a fire-risk assessment which takes into account all of the factors which are pertinent to an assessment of the fire hazard or fire risk of a particular end use.

1.6 The values stated in SI units are to be regarded as the standard. In cases where materials, products or equipment are available in inch-pound units only, SI units are omitted.

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

D1193 Specification for Reagent Water

3. Terminology

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *spontaneous heating value (SHV)*—the maximum amount by which the temperature of the sample exceeds that of the reference when exposed at a given temperature in the standard apparatus.

3.2 *Symbols:*

t_S = temperature of sample side at any time during test, K,
 t_R = temperature of reference side at time t_S is measured, K,
 T_S = maximum temperature of sample chamber during test, K,

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

- T_R = temperature of reference chamber measured at same time that T_S is measured, K,
- Δt = $t_S - t_R$,
- ΔT = $T_S - T_R$,
- B_R = equilibrium temperature of reference side during blank run, K,
- B_S = equilibrium temperature of sample side during blank run, K,
- ΔT_B = $B_S - B_R$ = instrumental blank,
- Δt_C = $\Delta t - (B_S - B_R) = \Delta t - \Delta T_B$, and
- ΔT_C = $\Delta T - (B_S - B_R) = \Delta T - \Delta T_B$ = spontaneous heating value.

4. Summary of Test Method

4.1 The sample is supported on surgical gauze and placed in a heated chamber which is open to the air at the top. The temperature of the sample, thus prepared, is compared to that of an equal reference quantity of surgical gauze contained in an identical chamber. The amount by which the temperature of the sample exceeds that of the reference is taken as an index of the spontaneous heating value of the sample. Tests may be conducted for durations of 4 to 72 h or longer if desired.

4.1.1 Any convenient, inert, fibrous substrate of adequate absorbency may be substituted for surgical gauze as required. Any such substitution shall be reported with the spontaneous heating value so obtained.

5. Significance and Use

5.1 The spontaneous heating value of a substance is a measure of the ability of that substance to undergo self-heating reactions while supported by cellulosic or other fibrous material in air. It is an index of the autoignition tendency of the substance under such conditions.

6. Apparatus

- 6.1 *Spontaneous Heating Apparatus*—See Fig. 1 and Fig. 2.
- 6.2 *Thermocouples*, 30-gage, iron-constantan, Type J. Two are required.
- 6.3 *Strip Chart Temperature Recorder*, two-channel or multipoint, capable of 0.5 K resolution at test temperature.
- 6.4 *Hot Plate*, capable of uniformly heating entire bottom surface of spontaneous heating apparatus.

7. Materials

- 7.1 *Cotton Gauze*, surgical.
- 7.2 *Water*, conforming to Specification D1193, Type III.

8. Procedure

8.1 Determination of Instrumental Blank:

8.1.1 Assemble the spontaneous heating apparatus and place 2000 mL of distilled water in the boiling chamber. Heat the apparatus until continuous refluxing occurs.

8.1.1.1 When test temperatures higher than that obtained by the refluxing of water in the test apparatus are desired, reagent grade ethylene glycol or any other suitable pure compound may be substituted for water. Report any such substitutions with the test data.

8.1.2 Pack the sample and reference containers (screen baskets) with 20 g of rolled cotton gauze. Insert a thermocouple in the center of the gauze mass in each container and place both in the apparatus.

NOTE 1—When considerable variation in temperature from the norm exists, an additional thermocouple may be necessary to measure the temperature of the bath.

8.1.3 Allow the system to attain thermal equilibrium and then continue heating for 4 h. Record temperature readings, B_R and B_S . Determine the average instrumental blank T_B , found

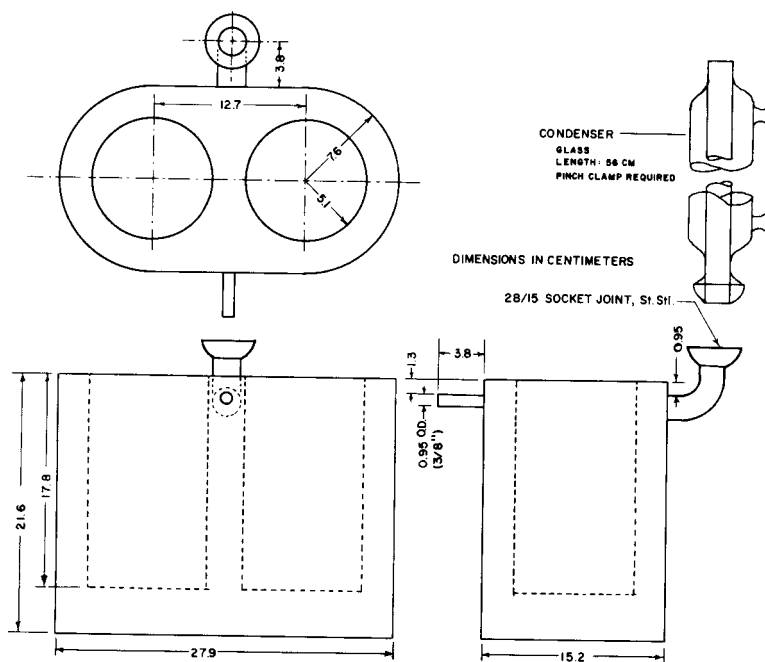


FIG. 1 Spontaneous Heating Apparatus (Copper Body)

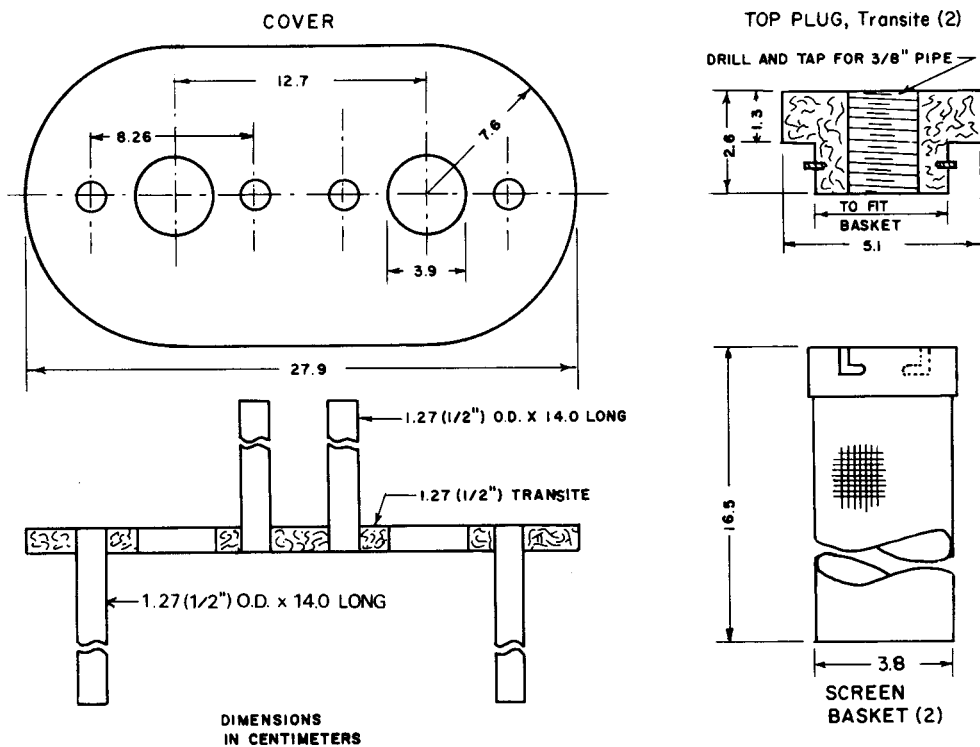


FIG. 2 Spontaneous Heating Apparatus

over the duration of the test from measurements of B_S and B_R made at 1/2-h intervals after establishment of thermal equilibrium.

8.2 Measurement of Spontaneous Heating Value:

8.2.1 Assemble the spontaneous heating apparatus and place 2000 mL of distilled water in the boiling chamber. Heat the apparatus until continuous refluxing occurs.

8.2.2 Pack the reference container (screen basket) with 20 g of freshly rolled cotton gauze.

8.2.3 For a liquid sample, saturate 20 g of freshly rolled cotton gauze with 10 g of liquid. For a solid sample record the particle size if appropriate, and roll 10 g of a solid sample in 20 g of fresh cotton gauze. Locate the sample as near as possible to the position of the thermocouple tip. Pack the sample and gauze in the sample container (screen basket).

NOTE 2—For simulation of self heating of oily wastes and similar materials, it may be necessary to use the sample to gauze ratios as high as 2:1.

NOTE 3—The SHV will tend to vary with the particle size of solid samples.

8.2.4 Samples that contain volatile components such as solvents in paint or coating materials may be conditioned to remove such solvents before being placed in the test apparatus. Conditioning will of necessity be determined by the nature of the sample and shall be described in the report.

8.2.5 Insert thermocouples in the sample and reference containers.

8.2.6 Allow the system to attain equilibrium (within 1.5 K (1.5°C)) and then continue heating for 4 h. Record temperature readings, t_R and t_S .

8.2.6.1 While the minimum duration shall be 4 h, extended test durations may be employed as required. The test duration shall be reported if a duration other than 4 h is employed.

9. Calculation and Report

9.1 Tabulate the values obtained for t_R and t_S and the temperature differences, Δt , which are associated with each as follows:

$$\Delta t = t_S - t_R \tag{1}$$

9.2 Calculate the temperature difference found at the maximum temperature, T_S , attained by the sample as follows:

$$\Delta T = T_S - T_R \tag{2}$$

9.3 Apply the instrument blank correction to the temperature differences at Δt and ΔT as follows:

$$\Delta t_C = \Delta t - (B_S - B_R) = \Delta t - \Delta T_B \tag{3}$$

$$\Delta T_C = \Delta T - (B_S - B_R) = \Delta T - \Delta T_B \tag{4}$$

9.4 Report the maximum value calculated for Δt_C or ΔT_C (usually ΔT_C) as the spontaneous heating value of the sample, SHV, at the initial reference temperature. For solid samples, report the particle size.

10. Precision and Bias

10.1 Because of the complex nature of Test Method D3523 for spontaneous heating values, and because of the expensive equipment involved, there is not a sufficient number of volunteers to permit a cooperative laboratory program for

determining the precision and bias. If the necessary volunteers can be obtained, a program will be undertaken at a later date.

11. Keywords

11.1 Differential Mackey Test; liquids; solids; spontaneous heating; spontaneous heating values

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).