



Standard Test Method for Sonic Shear Stability of Hydraulic Fluids¹

This standard is issued under the fixed designation D5621; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method covers the evaluation of the shear stability of hydraulic fluids in terms of the final viscosity that results from irradiating a sample of the hydraulic fluid in a sonic oscillator.

1.2 Evidence has been presented that a good correlation exists between the shear degradation that results from sonic oscillation and that obtained in a vane pump test procedure.²

1.3 This test method uses millimetres squared per second (mm^2/s), an SI unit, as the unit of viscosity. For information, the equivalent unit, cSt, is shown in parentheses.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*³

D445 Test Method for Kinematic Viscosity of Transparent and Opaque Liquids (and Calculation of Dynamic Viscosity)

D2603 Test Method for Sonic Shear Stability of Polymer-Containing Oils

D6022 Practice for Calculation of Permanent Shear Stability Index

3. Summary of Test Method

3.1 A convenient volume of hydraulic fluid is irradiated in a sonic oscillator for a period of time and the viscosities before and after irradiation are determined by Test Method **D445**. A

¹ This test method is under the jurisdiction of ASTM Committee **D02** on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee **D02.07** on Flow Properties.

Current edition approved Dec. 1, 2007. Published January 2008. Originally approved in 1994. Last previous edition approved in 2001 as D5621-01. DOI: 10.1520/D5621-07.

² Stambaugh, R. L., Kopko, R. J., and Roland, T. F., "Hydraulic Pump Performance—A Basis for Fluid Viscosity Classification", SAE Paper No. 901633. Available from Society of Automotive Engineers, 400 Commonwealth Dr., Warrendale, PA 15096.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

standard reference fluid containing a readily sheared polymer is run frequently to ensure that the equipment imparts a controlled amount of sonic energy to the sample.

3.2 The conditions to obtain the data for the precision statement were: 30 mL sample, 12.5 min calibration, and 40 min sample irradiation at 0°C jacket temperature.

4. Significance and Use

4.1 This test method was developed using Test Method **D2603-91**.

4.2 This test method permits the evaluation of shear stability with minimum interference from thermal and oxidative factors that may be present in some applications. It has been found applicable to fluids containing both readily sheared and shear-resistant polymers. Correlation with performance in the case of hydraulic applications has been established.

5. Apparatus

5.1 *Sonic Shear Unit*, fixed frequency oscillator and sonic horn.⁴

5.2 *Auxiliary Equipment*—To facilitate uniform performance, the following auxiliary equipment is recommended:

5.2.1 *Cooling Bath or Ice Bath*, to maintain a jacket temperature of 0°C.

5.2.2 *Griffin 50-mL Beaker*, borosilicate glass.

5.2.3 *Sonic-Insulated Box*, to enclose the sonic horn to reduce the ambient noise level produced by the sonic shear unit.

5.3 *Viscometer*, any viscometer and bath meeting the requirements of Test Method **D445**.

6. Reference Fluids

6.1 The reference fluid is ASTM Reference Fluid B,⁵ a petroleum oil containing a polymer capable of being broken down by turbulence at high rates of shear. This oil has a

⁴ In the round robin program, equipment from Sonic Systems, Inc., 109 Pheasant Run, Newtown, PA 18040 and Heat Systems Ultrasonic, Inc., 1938 New Highway, Farmingdale, NY 11735, were found to be satisfactory.

⁵ The sole source of supply of the fluid known to the committee at this time is RohMax USA, 723 Electronic Drive, Horsham, PA 19044-2228. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

*A Summary of Changes section appears at the end of this standard.

viscosity of about 13.6 mm²/s (cSt) at 40°C. The viscosity of a specific lot is supplied by the provider of that lot.

7. Calibration of Apparatus

7.1 The reference fluid provides a practical way to define the performance (severity level) of a sonic oscillator unit so that satisfactory comparison can be made between tests run on different days in the same unit and between tests run with different units.

7.2 The decrease in viscosity observed for a given hydraulic fluid on irradiation in an oscillator unit depends on a number of factors; these include sample volume, irradiation time, and oscillator power setting. Frequency of the generator is 23 ± 2 kHz. Typical power settings are in the range of 50 watts. Manual tuning of the oscillator-horn combination is also required in some instruments in order to ensure efficiency of energy coupling between the two units. The procedure described in 7.3 is recommended for establishing a reproducible performance level for a given unit.

7.3 Confirm and record the 40°C viscosity of the reference fluid. Introduce 30 mL (room temperature) of the reference fluid into the 50-mL Griffin beaker. Immerse the beaker in ice water or a constant temperature bath at 0°C until the sample fluid level is below the liquid level in the bath. The beaker should be maintained in a vertical position in the bath. Secure beaker in this position and condition the sample for 12.5 min before commencing irradiation. Immerse the sonic horn into the sample fluid until the tip is at least 10 mm below the surface of fluid (see Fig. 1) in order to ensure that the tip remains submerged during the test. Exercise care to avoid contact of the tip with the bottom of the beaker as this will shorten tip life. The horn should be placed in a vertical position in the fluid and centered in the beaker (a weighted ring stand may be used to support the horn in this position). True vertical positioning is not critical and is intended primarily to minimize liquid splashing during irradiation. Irradiate the fluid for 12.5 min at a preselected power setting. Determine the decrease in reference fluid viscosity measured at 40°C. Repeat as necessary to determine the proper power setting to produce a viscosity change at 40°C of 15.0 % (± 1 %). Use this power setting for subsequent test runs. Daily recalibration of the apparatus is required because the power setting required to produce a stated viscosity loss will probably vary from day to day. Experience with a given apparatus set will determine whether more frequent calibration is required. Calibration in this manner will ensure that repeatable severity levels are established.

8. Procedure

8.1 Clean the sonic horn using a lintless wiper and optional solvent and calibrate the apparatus as described in 7.3. Introduce 30 mL of the hydraulic fluid sample to be tested into a clean 50-mL Griffin beaker and immerse in the constant temperature bath at 0°C. The beaker should be in a vertical position. Allow the sample to equilibrate for 12.5 min. Immerse the sonic horn in the fluid as described in 7.3. Irradiate the sample for 40 min at exactly the same power setting

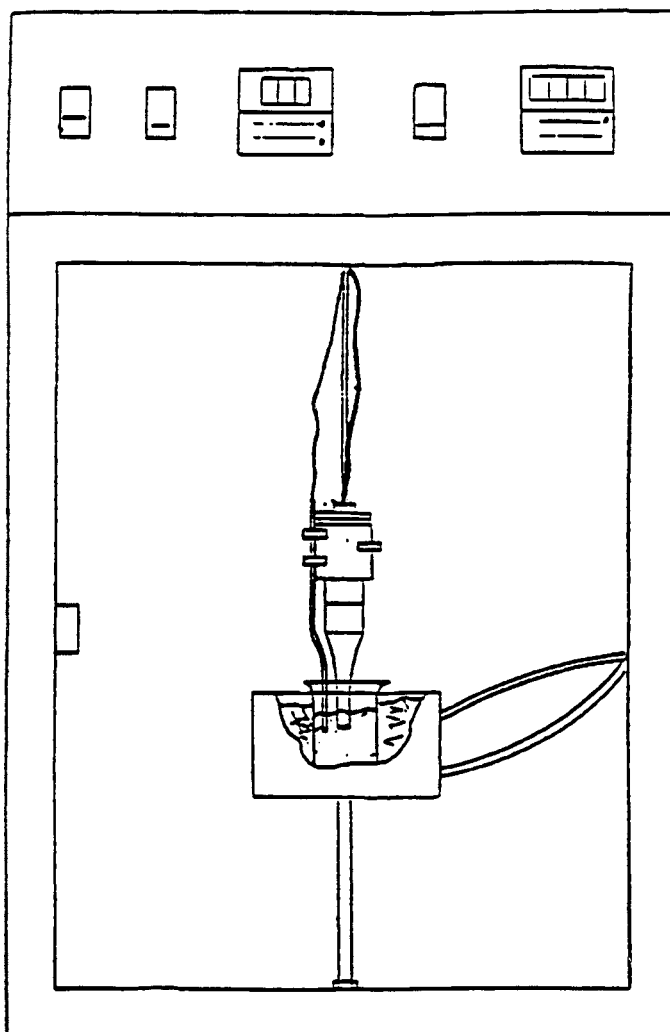


FIG. 1 Schematic of Sonic Probe Type Apparatus, Support Systems, Cabinet, and Power Supply

determined in 7.3. Upon completion of irradiation, remove the sample and clean the sonic horn in preparation for the next run.

8.2 Determine the viscosity of the sample by Test Method D445 before and after irradiation.

9. Report

9.1 Report the initial and irradiated 40°C viscosity of the hydraulic fluid.

9.2 In addition, the percent viscosity change may be calculated and reported. The percentage loss of viscosity is calculated as follows:

$$\text{Viscosity loss, \%} = [V_0 - V_f/V_0] \times 100 \quad (1)$$

where:

V_0 = viscosity of oil before irradiation, mm²/s (cSt), and
 V_f = viscosity of oil after irradiation, mm²/s (cSt).

9.3 The permanent shear stability index (PSSI) may also be calculated and reported in accordance with Practice D6022, provided the base fluid viscosity is known.

10. Precision and Bias ⁶

10.1 *Repeatability*—The difference between two independent irradiated viscosity results obtained by the same operator with the same apparatus under constant operating conditions on identical test material would, in the long run, in the normal and correct operation of the test method, differ from the mean by greater than 0.38 mm²/s (cSt) in only one case in twenty.

10.2 *Reproducibility*—The difference between two independent irradiated viscosity results obtained by different operators working in different laboratories on identical test material

⁶ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report D02-1337.

would, in the long run, in the normal and correct operation of the test method, differ from the mean by greater than 0.60 mm²/s (cSt) in only one case in twenty.

10.3 *Bias*—The bias of this test method has not been determined because there is insufficient data on the relevant reference (test) standard.

10.4 The precision of the percent viscosity loss or the Permanent Shear Stability Index may be estimated using the precisions of the individual measurements as stated here and in Test Method **D445**.

11. Keywords

11.1 hydraulic fluid; shear stability; sonic shear test; viscosity stable

SUMMARY OF CHANGES

Subcommittee D02.07 has identified the location of selected changes to this standard since the last issue (D5621–01) that may impact the use of this standard.

- (1) The user measures the viscosity of a hydraulic fluid after a sonic shear procedure defined in this test method.
- (2) In addition to reporting the viscosity after shear, a percent viscosity loss or a shear stability index may be calculated if the appropriate initial viscosity and the base oil viscosity (in the

case of the index) are known.

- (3) Added Practice **D6022** to **9.3** and the Referenced Documents.
- (4) Added **9.2**, **9.3**, and **10.4**.
- (5) Revised **3.1**, **9.1**, **10.1**, and **10.2**.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).