



# Standard Test Method for Measurement of Hindered Phenolic Antioxidant Content in Non-Zinc Turbine Oils by Linear Sweep Voltammetry<sup>1</sup>

This standard is issued under the fixed designation D6810; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers the voltammetric determination of hindered phenol antioxidants in new or in-service non-zinc turbine oils in concentrations from 0.0075 weight % up to concentrations found in new oils by measuring the amount of current flow at a specified voltage in the produced voltammogram.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

[D1193](#) Specification for Reagent Water

[D4057](#) Practice for Manual Sampling of Petroleum and Petroleum Products

[D4378](#) Practice for In-Service Monitoring of Mineral Turbine Oils for Steam and Gas Turbines

[D6224](#) Practice for In-Service Monitoring of Lubricating Oil for Auxiliary Power Plant Equipment

[D6447](#) Test Method for Hydroperoxide Number of Aviation Turbine Fuels by Voltammetric Analysis

[D6971](#) Test Method for Measurement of Hindered Phenolic and Aromatic Amine Antioxidant Content in Non-zinc Turbine Oils by Linear Sweep Voltammetry

## 3. Summary of Test Method

3.1 A measured quantity of sample is dispensed into a vial containing a measured quantity of alcohol-based electrolyte solution and containing a layer of sand. When the vial is


shaken, the hindered phenol antioxidants and other solution soluble oil components present in the sample are extracted into the solution and the remaining droplets suspended in the solution are agglomerated by the sand. The sand/droplet suspension is allowed to settle out and the hindered phenol antioxidants dissolved in the solution are quantified by voltammetric analysis. The results are calculated and reported as weight percent of antioxidant or as millimoles (mmol) of antioxidant per litre of sample for prepared and fresh oils and as a percent remaining antioxidant for used oils.

3.2 Voltammetric analysis is a technique that applies electro-analytic methods when a sample to be analyzed is mixed with an electrolyte and a solvent and placed within an electrolytic cell. Data is obtained by measuring the current passing through the cell as a function of the potential applied, and test results are based upon current, voltage and time relationships at the cell electrodes. The cell consists of a fluid container into which is mounted a small, easily polarized working electrode, and a large nonpolarizable reference electrode. The reference electrode should be massive relative to the working electrode so that its behavior remains essentially constant with the passage of small current; that is, it remains unpolarized during the analysis period. Additional electrodes, auxiliary electrodes, can be added to the electrode system to eliminate the effects of resistive drop for high resistance solutions. In performing a voltammetric analysis, the potential across the electrodes is varied linearly with time, and the resulting current is recorded as a function of the potential. As the increasing voltage is applied to the prepared sample within the cell, the various additive species under investigation within the oil are caused to electrochemically oxidize. The data recorded during this oxidation reaction can then be used to determine the remaining useful life of the oil type. A typical current-potential curve produced during the practice of the voltammetric test can be seen by reference to [Fig. 1](#). Initially, the applied potential produces an electrochemical reaction having a rate so slow that virtually no current flows through the cell. As the voltage is increased, as shown in [Fig. 1](#), the electro-active species (for example, substituted phenols) begin to oxidize at the working electrode surface, producing an anodic rise in the current. As the potential is further increased,

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee [D02](#) on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee [D02.09.0C](#) on Oxidation of Turbine Oils.

Current edition approved July 1, 2007. Published August 2007. Originally approved in 2002. Last previous edition approved in 2002 as D6810-02. DOI: 10.1520/D6810-07.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

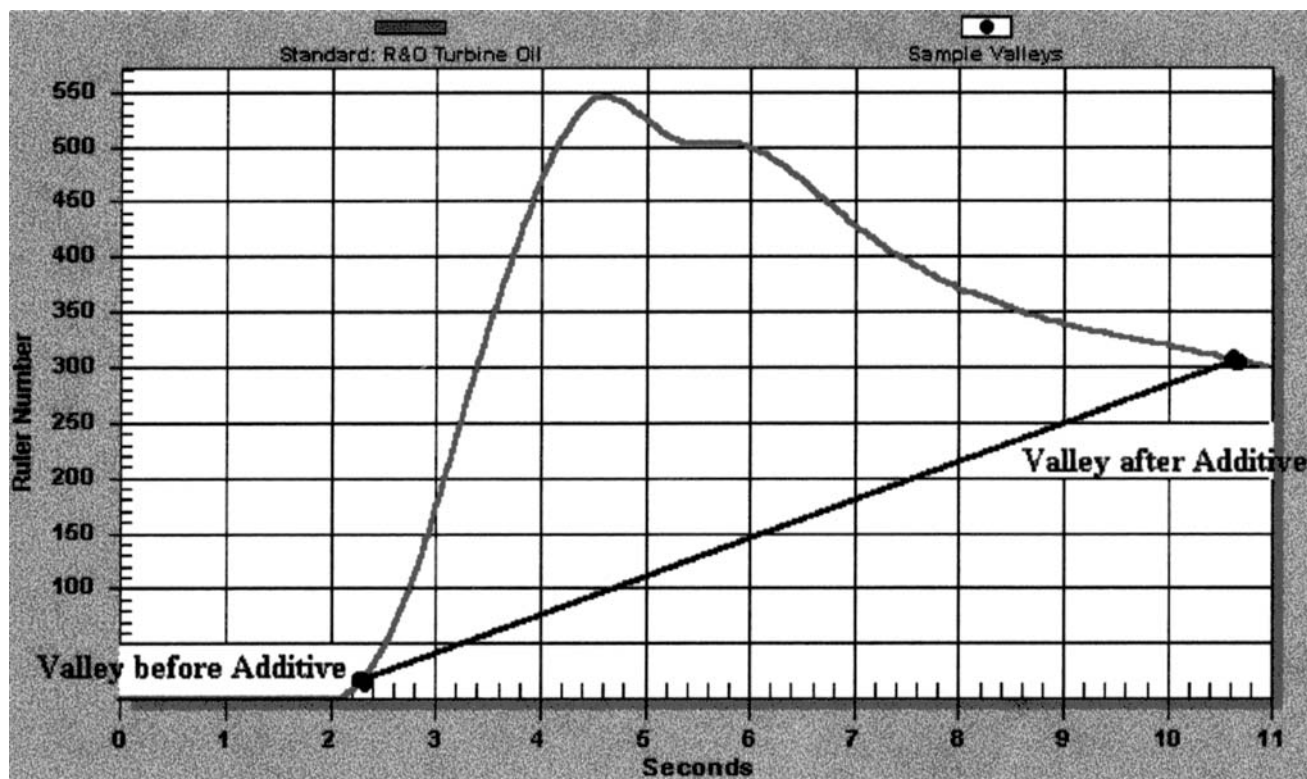

NOTE—x-axis = time (seconds) and y-axis is current (arbitrary units). Top line in Fig. 1 is voltammogram of a fresh R&O turbine oil showing valley indicator before and after standard.

FIG. 1 Hindered Phenol Voltammetric Response in Basic Test Solution with Blank Response Zeroed

the decrease in the electro-active species concentration at the electrode surface and the exponential increase of the oxidation rate lead to a maximum in the current-potential curve shown in Fig. 1.

#### 4. Significance and Use

4.1 The quantitative determination of hindered phenol antioxidants in a new turbine oil measures the amount of this material that has been added to the oil as protection against oxidation. Beside phenols, turbine oils can be formulated with other antioxidants such as amines which can extend the oil life. In used oil, the determination measures the amount of original (phenolic) antioxidant remaining after oxidation have reduced its initial concentration. This test method is not designed or intended to detect all of the antioxidant intermediates formed during the thermal and oxidative stressing of the oils, which are recognized as having some contribution to the remaining useful life of the used or in-service oil. Nor does it measure the overall stability of an oil, which is determined by the total contribution of all species present. Before making final judgment on the remaining useful life of the used oil, which might result in the replacement of the oil reservoir, it is advised to perform additional analytical techniques (in accordance with Practices D6224 and D4378), having the capability of measuring remaining oxidative life of the used oil.

4.1.1 This test method is applicable to non-zinc turbine oils. These are refined mineral oils containing rust and oxidation inhibitors, but not antiwear additives. This test method has not yet been established with sufficient precision for antiwear oils.

4.2 This test method is also suitable for manufacturing control and specification acceptance.


4.3 When a voltammetric analysis is obtained for a turbine oil inhibited with a typical hindered phenol antioxidant, there is an increase in the current of the produced voltammogram between 3-5 s (or 0.3 to 0.6 V applied voltage) (see Note 1) in the basic test solution (Fig. 1—x-axis 1 second = 0.1 V). Hindered phenol antioxidants detected by voltammetric analysis include, but are not limited to, 2,6-di-tert-butyl-4-methylphenol; 2,6-di-tert-butylphenol and 4,4'-methylenebis(2,6-di-tert-butylphenol).

NOTE 1—Voltages listed with respect to reference electrode. The voltammograms shown in Figs. 1 and 2 were obtained with a platinum reference electrode and a voltage scan rate of 0.1 V/s.

4.4 For non-zinc turbine oils containing aromatic (aryl) amine compounds (antioxidants and corrosion inhibitors), there is an increase in the current of the produced voltammogram between 7-11 s (0.7 to 1.1 V applied voltage in Fig. 2) (see Note 1) which does not interfere with the hindered phenol measurement in the basic test solution. For the measurement of these aromatic amine antioxidants, refer to Test Method D6971, where the neutral test solution shall be used.

#### 5. Apparatus

5.1 *Voltammetric Analyzer*—The instrument used to quantify the hindered phenol antioxidants is a voltammograph equipped with a three-electrode system and a digital or analog output. The combination electrode system consists of a glassy

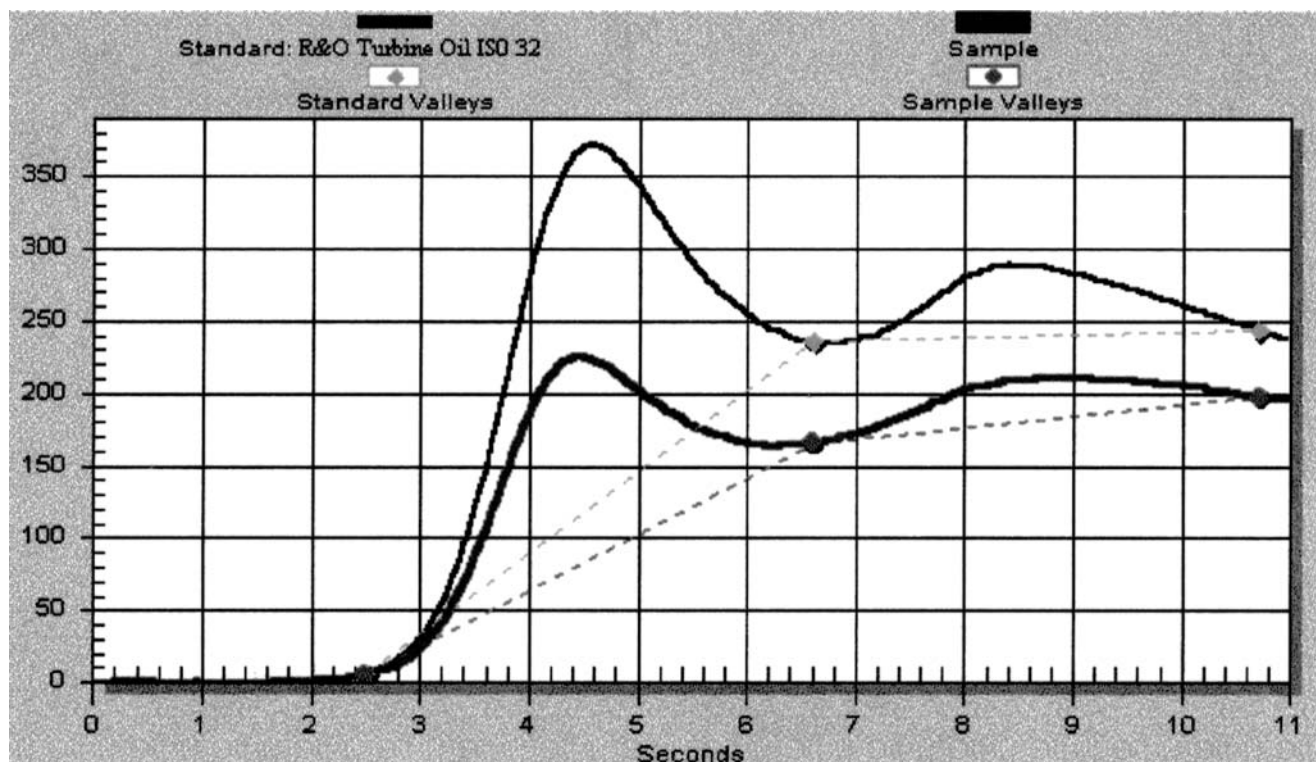

NOTE—x-axis = time (seconds) and y-axis is current (arbitrary units). Top line in Fig. 2 is fresh oil, and lower line is used oil.

FIG. 2 Amine and Hindered Phenols Peaks in the Basic Test Solution with Blank Response Zeroed

carbon disc (3-mm diameter) working electrode, a platinum wire (0.5-mm diameter) auxiliary electrode, and a platinum wire (0.5-mm diameter) reference electrode, as described in Test Method D6447. The voltammetric analyzer applies a linear voltage ramp (0 to -1.8 V range with respect to the reference electrode) at a rate of 0.01 to 0.5 V/s (0.1 optimum) to the auxiliary electrode. The current output of the working electrode is converted to voltage by the voltammetric analyzer, using the gain ratio of 1 V/20  $\mu$ A, and is outputted to an analog or digital recording device (0 to 1 V full scale) as shown in Figs. 1 and 2.

5.2 *Vortex Mixer*, with a 2800 to 3000 rpm motor and a pad suitable for mixing test tubes and vials.

5.3 *Pipette*, or equivalent, capable of delivering sample volumes required in this test method, from 0.10 to 0.50 mL.

5.4 *Solvent Dispenser*, or equivalent, capable of delivering volumes of analysis solution (see 7.3) required in this test method, such as 3.0 and 5.0 mL.

5.5 *Glass Vials*, with caps, 4 or 7-mL capacity; and containing 1 g of sand white quartz suitable for chromatography, within the size range of 200 to 300  $\pm$  100  $\mu$ m.

## 6. Sampling

6.1 Obtain the sample in accordance with Practice D4057.

## 7. Reagents

7.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society,

where such specifications are available.<sup>3</sup> Other grades may be used, provided it is first ascertained that the reagent is sufficiently pure to permit its use without lessening the accuracy of the determination.

7.2 *Purity of Water*—Unless otherwise specified, references to water that conforms to Specification D1193, Type II.

### 7.3 Analysis Materials:

7.3.1 *Alcohol Test Solution (Basic Test Solution)*—Proprietary yellow solution, ethanol solvent (1:10 distilled water/ethanol solution) containing a dissolved base electrolyte. (**Warning**—Corrosive, poison, flammable, skin irritant; harmful if inhaled.)


7.3.2 *Alcohol Cleansing Pads*—70 % isopropyl alcohol saturated cleansing pads.

## 8. Procedure

8.1 The voltammetric analyzer used in this test method gives linear results between 2 to 50 mmol for hindered phenols using an oil sample size of 0.40 and 5.0 mL of the analysis solvent. The corresponding range of weight percents depends on the molecular weight of the hindered phenol and the density of the base oil. For instance, the weight % range of 0.044 to 1.1 is equal to 2 to 50 mmol/L for a hindered phenol containing

<sup>3</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.



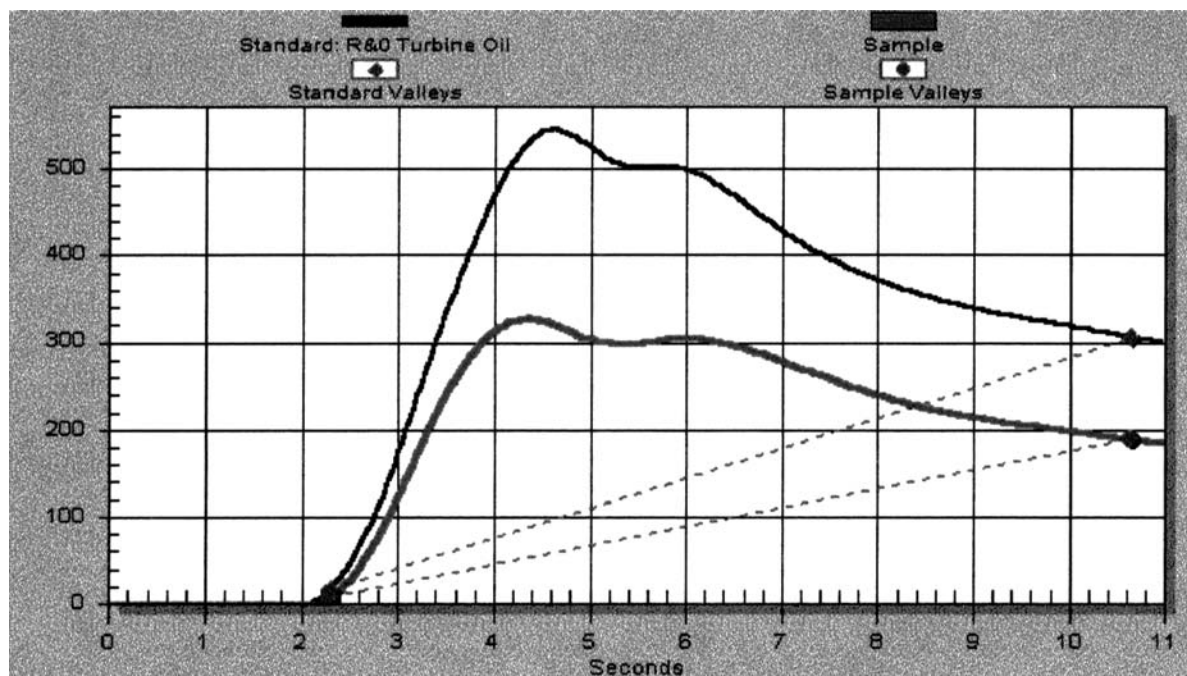

NOTE—Standard (top line) and sample used oil (lower line).

FIG. 3 Voltammetric Reading for a Used Oil Sample Comparing Hindered Phenols Peaks (in the Basic Test Solution)

one hydroxyl group and with a molecular weight of 220 g/mol (2,6-di-tert-butyl-4-methylphenol) and an oil density of 1 g/mL. Below 2 mmol, the noise to signal ratio becomes large decreasing the accuracy of the measurements. For measurements below 2 mmol or for fresh oils with high noise to signal ratios, the sample size should be increased to 0.60 mL and the volume of analysis solvent decreased to 3.0 mL.

8.2 *General Voltammetric Test Procedure*—The test procedure for voltammetric analysis will consist of the blank reading (calibration), followed by a standard reading and finally the test sample (in-service oil) reading.

8.2.1 *Blank Reading*—(0 mmol/L = 0 weight %).

8.2.1.1 *Definition*—The blank reading (voltammetric number) is a measurement of the analysis solution by itself. The blank measurement gives a reference number with no antioxidant present (the zero baseline).

8.2.2 *Standard Reading*—(30 to 150 mmol/L—weight % dependent on density of fresh oil and molecular weight of antioxidant).

8.2.2.1 *Definition*—The standard reading is a measurement of a fresh, unused oil (containing phenolic antioxidant) mixed with an appropriate analysis solvent. This measurement gives you a voltammetric reading (standard reading) that indicates the voltammetric response for the concentration hindered phenol antioxidant being analyzed for the oil being tested.

8.2.3 *Test Sample (In-Service Oil) Reading*:

8.2.3.1 *Definition*—The sample reading is a measurement of a fresh or in-service oil mixed with the same type of analysis solvent as the standard. This measurement will provide voltammetric readings that normally range between the blank and standard measurements, and reflect the concentration of hindered phenol antioxidant present (fresh oil) or remaining

(in-service oil) in the oil sample. Voltammetric readings for in-service oil will decrease as hindered phenol antioxidants are depleted.

8.3 *Voltammetric Reading*—After the operator has selected the valleys before and after the antioxidant peaks (as shown in Fig. 1), the software (R-DMS) will automatically identify and calculate the area above the baseline between the two valley indicators. This calculated area is then used for the test sample reading (in-service oil), which will be established by comparing the in-service oil area to its standard (see Fig. 3) and make remaining antioxidant calculations (see Section 9). If peak shifting is occurring, it is advised to repeat the voltammetric test after performing the cleaning of the electrode. If after this second test the peak shifting remains persistent, it is advised to drag the valley indicators manually to their shifted locations.

8.4 *Calibration (Blank Reading) Procedure*—Pipette 5.0 mL of analysis solution into a 7-mL vial or other suitable container containing 1 g of sand. Insert the electrode of the voltammetric analyzer into the analysis solution to wet the bottom surface of the electrode, remove, and rub dry the bottom electrode surface with a lint-free paper towel. Insert the electrode into the vial so that the bottom of the electrode is submerged in the analysis solution without resting on the sand layer on the bottom of the vial. Place the vial/probe upright into the rack or foam block for testing. Perform the voltammetric analysis (see 5.1). Record the voltammetric reading in the voltage range of the phenols, 0.3 to 0.6 V (see Note 1) in basic solution and Fig. 1. Remove the combination electrode from the blank solution and rub dry the bottom surface of the electrode with a lint free paper towel. Run at least two tests of the analysis solution to assure the electrode is clean and the minimal blank value has been obtained.

8.4.1 *Calibration Frequency*—Recalibration with freshly prepared blank solution can be performed before each testing session, or with the use of a new batch of test solutions.

8.5 *Standard and In-Service Oil Sample Preparation Procedures*:

8.5.1 *Preparing Solution Step*—Remove the seal and cap of the test solution vial. Pipette 5.0 mL of analysis solution into a 7-mL vial or other suitable container containing 1 g of sand. Pipette 0.40 mL of the selected oil sample also into the 7-mL vial.

8.5.2 For measurements below 2 mmol or for fresh oils with high noise to signal ratios, the sample size should be increased to 0.60 mL and the volume of analysis solvent decreased to 3.0 mL.

8.5.3 *Shaking Solution Step*—Cap the vial and shake vigorously using a vortex mixer for 20 s or by hand (between 50 and 60 shaking cycles/min), until sand is thoroughly mixed. Place the prepared oil solution upright in a rack or perforated foam block for a minimum time of 30 s to allow the sand to settle on the bottom of the vial with the oil.

8.5.4 *Cleaning Electrode Step*—Prepare the electrode for analysis by cleaning the electrode. Use an alcohol-cleansing pad to wet the bottom surface of the electrode. The bottom of the electrode must be dried immediately with a clean lens tissue (lint-free paper towel). The glassy carbon surface should always have a polished look before running a test. A glazed or cloudy look indicates the presence of a chemical film. If the probe tip is not cleaned properly, voltammetric readings can be distorted.

8.5.5 *Running Test Step*—Insert the electrode into the vial so that the bottom of the electrode is submerged in the analysis solution without resting on the sand layer on the bottom of the vial. Place the vial/probe upright into the rack or foam block for testing. Perform the voltammetric analysis (see 5.1) for hindered phenolic antioxidants. Record the valley to valley antioxidant reading in the voltage range of the phenols, 0.3 to 0.6 V (see Note 1) in the basic test solution (Fig. 1). Remove the combination electrode from the oil solution and repeat the cleaning procedure of the electrode. Run at least two tests (cleaning the electrode and shaking the standard for 10 s between tests) of the standard or in-service oil sample to ensure the value is stable and repeatable.

8.5.6 Make all measurements within 5 min after the initial mixing of the analysis solution, selected sample, and sand.

8.6 When the manufacturer of the oil is known, and the uninhibited base oil is available, use it to prepare the standards (mmol or weight percent antioxidant calculations). Prepare a standard containing in the range of 30 to 150 mmol/L of oil (0.5 to 3.0 weight %) of the selected phenolic antioxidant dissolved in an uninhibited base oil. The concentration should be selected to span the expected concentrations of the new and in-service oil samples.

8.7 Standard readings should be updated whenever new batches of lubricants are stocked, and periodically to monitor the amount of natural oxidation occurring in the stock during storage.

8.8 For fresh or in-service oils of unknown origin, use a typical fresh turbine oil as the standard (100 % remaining antioxidant calculations).

8.9 The analysis solution and scan time should be the same for the blank, standard, and in-service oil sample.

## 9. Calculations

9.1 *Percent Hindered Phenol Antioxidant Calculation*—If the hindered phenol antioxidant present in the oil sample is known, then the percent hindered phenol antioxidant in the sample can be calculated as follows:

$$\begin{aligned} \text{Percent of Hindered Phenol Antioxidant} = \\ \frac{\text{Sample Reading} - \text{Blank Reading}}{\text{Standard Reading} - \text{Blank Reading}} \times \\ \text{Percent Hindered Phenol Antioxidant of Standard} \end{aligned}$$

where:

reading = valley to valley area (see 8.3) for peak between 0.3 to 0.6 V (see Note 1).

9.2 *Molar Concentration of Hindered Phenol Antioxidant Calculation*—If the phenol hindered phenol antioxidant in the oil sample is unknown, then the millimoles of hindered phenol antioxidant in the sample can be calculated as follows:

$$\begin{aligned} \text{Concentration of Hindered Phenol Antioxidant, mmol/L of oil} = \\ \frac{\text{Sample Reading} - \text{Blank Reading}}{\text{Standard Reading} - \text{Blank Reading}} \times \end{aligned}$$

Hindered Phenol Antioxidant Concentration of Standard (mmol/L of oil)

where:

reading = valley to valley area (see 8.3) for peak between 0.3 to 0.6 V (see Note 1).

9.3 *Percent Remaining Hindered Phenol Antioxidant Calculation*—Calculate the percent remaining hindered phenol antioxidant in an in-service oil using the fresh oil as the 100 % standard with the following calculation:

$$\begin{aligned} \% \text{ Remaining Hindered Phenol Antioxidant} = \\ \frac{\text{Sample Reading} - \text{Blank Reading}}{\text{Standard Reading} - \text{Blank Reading}} \times 100 \% \end{aligned}$$

where:

reading = valley to valley area (see 8.3) for peak between 0.3 to 0.6 V (see Note 1).

## 10. Precision and Bias <sup>4</sup>

10.1 The following criteria should be used for judging the acceptability of results (95 % of confidence).

10.1.1 *Repeatability*—The difference between concurrent test results obtained by the same operator with the same apparatus under constant operating conditions on identical test materials, would, in the long run, and in the normal and correct operation of this test method, exceed the following values only in 1 case in 20:

<sup>4</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1548.

$$\text{Repeatability} = 0.7779 \times (x + 2)^{0.5} \%$$

where:  
 $x$  = mean value.

10.1.2 *Reproducibility*—The difference between two single and independent results, obtained by different operators working in different laboratories on identical test material, would, in the long run, and in the normal and correct operation of this test method, exceed the following values only in 1 case in 20:

$$\text{Reproducibility} = 1.830 \times (x + 2)^{0.5} \%$$

where:  
 $x$  = mean value.

## 11. Keywords

11.1 2,6-di-tert-butyl-4methylphenol; 2,6-di-tert-butylphenol; aromatic amines; hindered phenol antioxidant; in-service oils; linear sweep voltammetry; non-zinc turbine oils; turbine oil

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).*