



Standard Test Method for Gross Calorific Value of Coal and Coke¹

This standard is issued under the fixed designation D5865; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method pertains to the determination of the gross calorific value of coal and coke by either an isoperibol or adiabatic bomb calorimeter.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* Specific hazard statements are given in Section 8.

2. Referenced Documents

2.1 ASTM Standards:²

- D121 Terminology of Coal and Coke
- D346 Practice for Collection and Preparation of Coke Samples for Laboratory Analysis
- D388 Classification of Coals by Rank
- D1193 Specification for Reagent Water
- D2013 Practice for Preparing Coal Samples for Analysis
- D3173 Test Method for Moisture in the Analysis Sample of Coal and Coke
- D3177 Test Methods for Total Sulfur in the Analysis Sample of Coal and Coke
- D3180 Practice for Calculating Coal and Coke Analyses from As-Determined to Different Bases
- D4239 Test Method for Sulfur in the Analysis Sample of Coal and Coke Using High-Temperature Tube Furnace Combustion
- D5142 Test Methods for Proximate Analysis of the Analysis Sample of Coal and Coke by Instrumental Procedures
- E144 Practice for Safe Use of Oxygen Combustion Bombs

- E178 Practice for Dealing With Outlying Observations
- E882 Guide for Accountability and Quality Control in the Chemical Analysis Laboratory
- E2251 Specification for Liquid-in-Glass ASTM Thermometers with Low-Hazard Precision Liquids

3. Terminology

3.1 Definitions:

3.1.1 *adiabatic calorimeter*—a calorimeter that operates in the adiabatic mode and may or may not use a microprocessor. The initial temperature before initiating the combustion and the final temperatures are recorded by the operator or the microprocessor.

3.1.2 *automated calorimeter*—a calorimeter which has a microprocessor that takes the thermometric readings and calculates the Calibration Value and the Heat of Combustion Values.

3.1.3 *British thermal unit [Btu]*—is the amount of heat required to raise the temperature of one pound - mass [lbm] of liquid water at one atmosphere pressure one degree Fahrenheit at a stated temperature. The results of combustion calorimetric tests of fuels for steam power plants may be expressed in terms of the 1956 International Steam Table calorie (I.T. cal) which is defined by the relation, 1 I.T. cal = 4.1868 J. The Btu used in modern steam tables is defined by the means of the relation, 1 I.T. cal / g = 1.8 I.T. Btu / lb. Thus, 1 I.T. Btu / lb = 2.326 J / g.

3.1.4 *calorific value*—the heat produced by combustion of a unit quantity of a substance under specified conditions.

3.1.5 *calorimeter*—a device for measuring calorific value consisting of a bomb, its contents, a vessel for holding the bomb, temperature measuring devices, ignition leads, water, stirrer, and a jacket maintained at specified temperature conditions.

3.1.6 *gross calorific value (gross heat of combustion at constant volume), Q_v (gross)*—the heat produced by complete combustion of a substance at constant volume with all water formed condensed to a liquid.

3.1.7 *heat of formation*—the change in heat content resulting from the formation of 1 mole of a substance from its elements at constant pressure.

3.1.8 *isoperibol calorimeter*—a calorimeter that operates in the isoperibol mode and uses a microprocessor to record the initial and final temperatures and make the appropriate heat leak

¹ This test method is under the jurisdiction of ASTM Committee D05 on Coal and Coke and is the direct responsibility of Subcommittee D05.21 on Methods of Analysis.

Current edition approved May 1, 2010. Published July 2010. Originally approved in 1995. Last previous edition approved in 2010 as D5865 – 10. DOI: 10.1520/D5865-10A.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard.

corrections during the temperature rise. It determines when the calorimeter is in equilibrium and ignites the sample and determines when the calorimeter has reached equilibrium after ignition.

3.1.9 *net calorific value (net heat of combustion at constant pressure), Q_p (net)*—the heat produced by combustion of a substance at a constant pressure of 0.1 MPa (1 atm), with any water formed remaining as vapor.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *corrected temperature rise*—the calorimeter temperature change caused by the process that occurs inside the bomb corrected for various effects.

3.2.2 *heat capacity*—the energy required to raise the temperature of the calorimeter one arbitrary unit.

3.2.2.1 *Discussion*—The heat capacity can also be referred to as the energy equivalent or water equivalent of the calorimeter.

4. Summary of Test Method

4.1 The heat capacity of the calorimeter is determined by burning a specified mass of benzoic acid in oxygen. A comparable amount of the analysis sample is burned under the same conditions in the calorimeter. The calorific value of the analysis sample is computed by multiplying the corrected temperature rise, adjusted for extraneous heat effects, by the heat capacity and dividing by the mass of the sample.

NOTE 1—Oxidation of coal after sampling can result in a reduction of calorific value. In particular, lignite and sub-bituminous rank coal samples may experience greater oxidation effects than samples of higher rank coals. Unnecessary exposure of the samples to the air for the time of sampling or delay in analysis should be avoided.

5. Significance and Use

5.1 The gross calorific value can be used to compute the total calorific content of the quantity of coal or coke represented by the sample for payment purposes.

5.2 The gross calorific value can be used for computing the calorific value versus sulfur content to determine whether the coal meets regulatory requirements for industrial fuels.

5.3 The gross calorific value can be used to evaluate the effectiveness of beneficiation processes.

5.4 The gross calorific value can be required to classify coals according to Classification **D388**.

6. Apparatus and Facilities

6.1 *Test Area*—An area free from drafts, shielded from direct sunlight and other radiation sources. Thermostatic control of room temperature and controlled relative humidity are desirable.

6.2 *Combustion Bomb*—Constructed of materials that are not affected by the combustion process or the products formed to introduce measurable heat input or alteration of end products. The bomb shall be designed so that all liquid combustion products can be completely recovered by washing the inner surfaces. There shall be no gas leakage. The bomb shall be capable of withstanding a hydrostatic pressure test to 20 MPa (3000 psig) at room temperature without stressing any part beyond its specified elastic limit.

6.3 *Balance*—A laboratory balance capable of weighing the analysis sample to the nearest 0.0001 g. The balance shall be checked weekly, at a minimum, for accuracy.

6.4 *Calorimeter Vessel*—Made of metal with a tarnish-resistant coating, with all outer surfaces highly polished. Its size shall be such that the bomb is completely immersed in water during a determination. A stirrer shall be provided for uniform mixing of the water. The immersed portion of the stirrer shall be accessible to the outside through a coupler of low thermal conductivity. The stirrer speed shall remain constant to minimize any temperature variations due to stirring. Continuous stirring for 10 min shall not raise the calorimeter temperature more than 0.01°C when starting with identical temperatures in the calorimeter, test area and jacket. For calorimeters having a bucket it can be a separate component or integral component of the bomb. The vessel shall be of such construction that the environment of the calorimeter's entire outer boundaries can be maintained at a uniform temperature.

6.5 *Jacket*—A container with the inner perimeter maintained at constant temperature $\pm 0.1^\circ\text{C}$ (isoperibol) or at the same temperature $\pm 0.1^\circ\text{C}$ as the calorimeter vessel (adiabatic) during the test. To minimize convection, the sides, top and bottom of the calorimeter vessel shall not be more than 10 mm from the inner surface of the jacket. Mechanical supports for the calorimeter vessel shall be of low thermal conductivity.

6.6 *Thermometers:*

6.6.1 *Platinum resistance or thermistor thermometers*—shall be capable of measuring to the nearest 0.0001°C. These types of thermometers consist of two major subsystems. The first and most obvious is the temperature sensing probe itself. The second and equally important aspect is the measurement subsystem. For both subsystems, the relationship between the thermometer resistance and temperature shall be well characterized. The absolute temperature shall be known to $\pm 0.1^\circ\text{C}$ at the temperature of the calorimetric measurement.

6.6.2 Assessing the valid working range of the calorimeter, as outlined in **10.9**, is sufficient to demonstrate that all important aspects of the calorimeter functionality, including the thermometry, are in good working order. The traceability of the heat of combustion measurement is governed by the traceability of the heat of combustion of the benzoic acid calibrant in addition to meeting the aforementioned criteria.

6.6.3 *Liquid-in-Glass Thermometers*—Conforming to the requirements for thermometers S56C, S116C, or S117C as prescribed in Specification **E2251**.

6.6.3.1 *Thermometer Accessories*—A magnifier is required for reading liquid-in-glass thermometers to one tenth of the smallest scale division. The magnifier shall have a lens and holder designed so as to minimize errors as a result of parallax.

6.6.4

6.7 *Sample Holder*—An open crucible of platinum, quartz, or base metal alloy. Before use in the calorimeter, heat treat base metal crucibles for a minimum of 4 h at 500°C to ensure the crucible surface is completely oxidized. Base metal alloy crucibles are acceptable, if after three preliminary firings, the weight does not change by more than 0.0001 g.

6.8 *Ignition Fuse*—Ignition fuse of 100-mm length and 0.16-mm (No. 34 B&S gauge) diameter or smaller. Nickel-chromium alloy (Chromel C) alloy, cotton thread, or iron wire are acceptable. Platinum or palladium wire, 0.10-mm diameter (No. 38 B&S gauge), can be used provided constant ignition energy is supplied. Use the same type and length (or mass) of ignition fuse for calorific value determinations as used for standardization.

6.9 *Ignition Circuit*—A 6- to 30-V alternating or direct current is required for ignition purposes. A step-down transformer connected to an alternating current circuit, capacitors, or batteries can be used. For manually operated calorimeters, the ignition circuit switch shall be of the momentary double-contact type, normally open except when held closed by the operator. An ammeter or pilot light can be used in the circuit to indicate when current is flowing.

6.10 *Controller*—For automated calorimeters, capable of charging the bomb; filling the calorimeter vessel; firing the ignition circuit; recording calorimeter temperatures before, during, and after the test; recording the balance weights; and carrying out all necessary corrections and calculations.

6.11 *Crucible Liner*—Quartz fiber or alundum for lining the crucible to promote complete combustion of samples that do not burn completely during the determination of the calorific value.³

7. Reagents

7.1 *Reagent Water*—Conforming to conductivity requirements for Type II of Specification **D1193** for preparation of reagents and washing of the bomb interior.

7.2 *Purity of Reagents*—Use reagent grade chemicals conforming to the specification of the Committee on Analytical Reagents of the American Chemical Society in all tests.⁴

7.3 *Benzoic Acid—Standard (C₆H₅COOH)*—Pellets made from benzoic acid available from the National Institute of Standards and Technology (NIST) or benzoic acid calibrated against NIST standard material. The calorific value of benzoic acid, for use in the calibration calculations, shall be traceable to a recognized certificate value.

7.4 *Oxygen*—Manufactured from liquid air, guaranteed to be greater than 99.5 % pure, and free of combustible matter. Oxygen made by the electrolytic process contains small amounts of hydrogen rendering it unfit unless purified by passage over copper oxide at 500°C.

7.5 *Titration Indicator*—Methyl orange, methyl red, or methyl purple for indicating the end point when titrating the acid formed during combustion. The same indicator shall be used for both calibration and calorific value determinations.

7.6 *Standard Solution*—Sodium carbonate (Na₂CO₃) or other suitable standard solution. Dissolve 3.757 g of sodium

carbonate, dried for 24 h at 105°C in water, and dilute to 1 L. One millilitre of this solution is equivalent to 4.2 J (1.0 calorie) in the acid titration.

8. Hazards

8.1 The following precautions are recommended for safe calorimeter operation. Additional precautions are noted in Practice **E144**. Also consult the calorimeter equipment manufacturer's installation and operating instructions before using the calorimeter.

8.1.1 The mass of sample and any combustion aid as well as the pressure of the oxygen admitted to the bomb shall not exceed the bomb manufacturer's specifications.

8.1.2 Inspect the bomb parts carefully after each use. Replace cracked or significantly worn parts. Replace O-rings and valve seats in accordance with manufacturer's instruction. For more details, consult the manufacturer.

8.1.3 Equip the oxygen supply cylinder with an approved type of safety device, such as a relief valve, in addition to the needle valve and pressure gauge used in regulating the oxygen feed to the bomb. Valves, gauges, and gaskets shall meet industry safety codes. Suitable reducing valves and adapters for 3- to 4-MPa (300- to 500-psig) discharge pressure can be obtained from commercial sources of compressed gas equipment. Check the pressure gauge annually for accuracy or after any accidental over pressures that reach maximum gauge pressure.

8.1.4 During ignition of a sample, the operator shall not extend any portion of the body over the calorimeter.

8.1.5 Do not fire the bomb if the bomb has been dropped or turned over after loading.

8.1.6 Do not fire the bomb if there is evidence of gas leakage when the bomb is submerged in the calorimeter vessel.

8.1.7 For manually operated calorimeters, the ignition switch shall be depressed only long enough to fire the charge.

9. Sample

9.1 The analysis sample is the material pulverized to pass 250- μ m (No. 60) sieve, prepared in accordance with either Practice **D346** for coke or Method **D2013** for coal.

10. Determination of the Heat Capacity of the Calorimeter

10.1 *Sample*—Weigh 0.8 to 1.2 g of benzoic acid into a sample holder. Record sample weight to the nearest 0.0001 g.

10.2 Preparation of Bomb:

10.2.1 Rinse the bomb with water to wet internal seals and surface areas of the bomb or precondition the calorimeter according to the manufacturer's instructions. Add 1.0 mL of water to the bomb before assembly.

10.2.2 Connect a measured fuse in accordance with manufacturer's guidelines.

10.2.3 Assemble the bomb. Admit oxygen to the bomb to a consistent pressure of between 2 and 3 MPa (20 and 30 atm). The same pressure is used for each heat capacity run. Control oxygen flow to the bomb so as not to blow material from the sample holder. If the pressure exceeds the specified pressure, detach the filling connection and exhaust the bomb. Discard the sample.

³ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D05-1025.

⁴ *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

10.3 Preparation of Calorimeter:

10.3.1 Fill the calorimeter vessel with water at a temperature not more than 2°C below room temperature and place the assembled bomb in the calorimeter. Check that no oxygen bubbles are leaking from the bomb. If there is evidence of leakage, remove and exhaust the bomb. Discard the sample.

10.3.2 The mass of water used for each test run shall be $M \pm 0.5$ g where M is a fixed mass of water. Devices used to supply the required mass of water on a volumetric basis shall be adjusted when necessary to compensate for change in the density of water with temperature.

10.3.3 With the calorimeter vessel positioned in the jacket start the stirrers.

10.4 Temperature Observations Automated Calorimeters:

10.4.1 *Stabilization*—The calorimeter vessel's temperature shall remain stable over a period of 30 s before firing. The stability shall be $\pm 0.001^\circ\text{C}$ for an adiabatic calorimeters and $\pm 0.001^\circ\text{C/s}$ or less for an isoperibol calorimeter.

10.4.2 *Extrapolation Method*—Fire the charge, record the temperature rise. The test can be terminated when the observed thermal curve matches a thermal curve which allows extrapolation to a final temperature with a maximum uncertainty of $\pm 0.002^\circ\text{C}$.

10.4.3 *Full Development Method*—Fire the charge and record the temperature rise until the temperature has stabilized for a period of 30 s in accordance with the stability requirements specified in 10.4.1.

10.5 Temperature Observations Manual Calorimeters:

10.5.1 When using ASTM Thermometers S56C, estimate all readings to the nearest 0.002°C . When using ASTM Thermometers S116C, or S117C, estimate readings to 0.001°C and 25- Ω resistance thermometer readings to the nearest 0.0001Ω . Tap or vibrate liquid-in-glass thermometers just before reading to avoid errors caused by liquid sticking to the walls of the capillary.

10.5.2 Allow 5 min for the temperature of the calorimeter vessel to stabilize. Adjust the jacket temperature to match the calorimeter vessel temperature within 0.01°C and maintain for 3 min.

10.5.3 Fire the charge. Record the time as a and the temperature as t_a .

10.5.4 For adiabatic calorimeters adjust the jacket temperature to match that of the calorimeter vessel temperature during the period of the rise. Keep the two temperatures as equal as possible during the period of rapid rise. Adjust to within 0.01°C when approaching the final stabilization temperature. Record subsequent readings at intervals no greater than 1 min until three successive readings do not differ by more than $\pm 0.001^\circ\text{C}$. Record the first reading after the rate of change has stabilized as the final temperature t_c and the time of this reading as c . For isoperibol calorimeters, when approaching the final stabilization temperature, record readings until three successive readings do not differ by more than 0.001°C per min. Record the first reading after the rate of change has stabilized as the final temperature as t_c and the time of this reading as c .

10.5.5 Open the calorimeter and remove the bomb. Release the pressure at a uniform rate such that the operation will not

be less than 1 min. Open the bomb and examine the bomb interior. Discard the test if unburned sample or sooty deposits are found.

10.6 Thermochemical Corrections (see Appendix X1):

10.6.1 *Acid Correction (see X1.1)*—One may use either the titration (10.6.1.1) or calculated titration (10.6.1.2) procedure for coal and coke samples.

10.6.1.1 *Titration Method*—Wash the interior of the bomb with distilled water containing the titration indicator (see 7.5) until the washings are free of acid and combine with the rinse of the capsule. Titrate the washings with the standard solutions (see 7.6) using a titration indicator, or a pH or millivolt meter. The number of millilitres of standard Na_2CO_3 used in the titration shall be taken as $e1$.

10.6.1.2 *Calculated Nitric Acid Method*—For test samples that contain no nitrogen, the nitric acid formed in the bomb during the combustion process is derived from the nitrogen in the air that occupies the bomb prior to pressurizing it with oxygen. The quantity of nitric acid formed is a function of the volume of the bomb, the oxygen filling pressure and the quantity of energy released in the bomb during a test. For a given bomb and filling pressure, the relationship between the amount of nitric acid formed and the energy released can be determined using the following procedure. The calorimeter should be tested using one-gram pellets of benzoic acid when the bomb volume is nominally 340 milliliters. If the bomb volume differs significantly from 340 ml, the sample weight used should be adjusted as required in order to comply with the bomb manufacturer's safe operating guidelines. Tests should be run in duplicate. Determine the nitric acid correction by titrating the bomb washings as outlined in 10.6.1.1. Divide the correction obtained ($e1$) by the amount of energy released in the bomb for the corresponding test. The energy contribution from the ignition fuse ($e2$) is usually small ($<1\%$ of the total energy released) and may be ignored. The average value of this ratio is used to establish a factor (NAF) that allows the nitric acid correction to be determined for any arbitrary energy release.

$$e1 = (\text{NAF}) * \text{energy released for the test} \quad (1)$$

Example:

The nitric acid correction for a 340-ml oxygen bomb is found to be 41.9 J (10.0 calories) when the released energy corresponds to that liberated by one gram of benzoic acid, 26.45 kJ (6318 calories). The ratio of these quantities is 1.58 J per 1000 joules of released energy or 1.58 calories per 1000 calories of released energy. The nitric acid correction for any calorimetric test can then be expressed as follows:

$$e1 = 1.58 * \text{energy released for the test (kJ or kcal)} \quad (2)$$

For a given calorimeter, the energy released in the bomb during a test for the purposes of calculating the nitric acid correction ($e1$) may be expressed as the product of the temperature rise for the test and the effective calorimeter heat capacity or calorimeter calibration factor.⁵

⁵ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D05-1028, "Interlaboratory Study for the Use of Calculated Nitric Acid Correction".

TABLE 1 Calibration Measurements

Run Number	Column A	Column B
	Heat Capacity J/C	Difference from Average Squared
1	10258	20
2	10249	20
3	10270	272
4	10254	0
5	10245	72
6	10249	20
7	10241	156
8	10266	156
9	10258	20
10	10245	72
Sum	102535	811
Average	10254	Sum Column A /10
Variance (s ²)	90	Sum Column B /9
Standard Deviation(s)	9	Sqrt (Variance)
Relative Standard Deviation (RSD)	0.09%	s/Average * 100

$$e1 = (1.58 / 1000) * E * t \quad (3)$$

The calculated nitric acid method can be applied to samples containing up to 2% nitrogen without introducing a significant error in the resulting heat of combustion value.

10.6.2 *Fuse Correction (see X1.3)*—Determine the fuse correction using one of the two alternatives:

10.6.2.1 Measure the combined pieces of unburned ignition fuse and subtract from the original length to determine the fuse consumed in firing according to Eq 4.

$$e2 = K_l \times l \quad (4)$$

where:

$e2$ = the correction for the heat of combustion of the firing fuse,

l = the length of fuse consumed during combustion,

K_l = 0.96 J/mm (0.23 cal/mm) for No. 34 B&S gauge Chromel C,

K_l = 1.13 J/mm (0.27 cal/mm) for No. 34 B&S gauge iron wire, and

K_l = 0.00 J/mm for platinum or palladium wire provided the ignition energy is constant.

or;

10.6.2.2 Weigh the combined pieces of unburned fuse and subtract from the original weight to determine the weight in milligrams of the fuse consumed in firing (m). Remove any ball of oxidized metal from the ends before weighing.

$$e2 = K_m \times m \quad (5)$$

where:

$e2$ = the correction for the heat of combustion of the firing fuse,

m = the weight in mg of fuse consumed during combustion,

K_m = 5.9 J/mg (1.4 cal/mg) for No. 34 B&S gauge Chromel C,

K_m = 7.5 J/mg (1.8 cal/mg) for No. 34 B&S gauge iron wire, and

K_m = 0.00 J/mg for platinum or palladium wire provided the ignition energy is constant.

When cotton thread is used, employ the correction in J recommended by the instrument manufacturer.

10.7 *Calculation of the Corrected Temperature Rise*—Compute the corrected temperature rise, t , as follows:

$$t = t_c - t_a + C_e + C_r \quad (6)$$

where:

t = corrected temperature rise, °C;

t_a = initial temperature reading at time of firing;

t_c = final temperature reading;

C_e = thermometer, emergent stem correction (see Eq A1.6 or Eq A1.8);

C_r = radiation correction (see Eq A1.1 or Eq A1.2).

10.7.1 The temperature rise in isoperibol calorimeters require a radiation correction.

10.8 *Calculation of the Heat Capacity*—Calculate the heat capacity (E) of the calorimeter using the following equation:

$$E = [(H_c \times m) + e1 + e2]/t \quad (7)$$

where:

E = the calorimeter heat capacity, J/°C;

H_c = heat of combustion of benzoic acid, as stated in the certificate, J/g;

m = mass of benzoic acid, g;

$e1$ = acid correction from 10.6.1 from either the titration method (10.6.1.1) or the calculated titration (10.6.1.2);

$e2$ = fuse correction from 10.6.2, J; and

t = corrected temperature rise from 10.7, °C.

10.8.1 Using the procedures described in 10.1-10.8 complete a total of ten acceptable test runs. An individual test shall be rejected only if there is evidence of incomplete combustion.

10.8.2 The precision of ten acceptable calibration test runs shall have a relative standard deviation (RSD) no greater than 0.17%. If after considering the possibility of outliers using criteria established in Practice E178, this limit is not met, one should review operation of the calorimeter for any assignable cause. Operating deficiencies should be corrected before performing additional calibration measurements as required. **Table**

1 provides an example summary of a series of calibration tests. The formulas used to arrive at the mean value and relative standard deviation are independent of the units used for the calibration measurements.

10.9 Valid Working Range for the Calibration of the Calorimeter:

10.9.1 It is a generally accepted principle of reliable analysis that instruments should be calibrated over the full range of measurement and that measurements be restricted to the range calibrated. It is not good practice to report extrapolated data obtained outside the range of calibration. The range or reliable calibration can be considered as the range of reliable measurement and vice versa.

10.9.2 It should be possible to vary the amount of benzoic acid calibrant by at least $\pm 25\%$ without observing a significant trend in the values obtained for the effective heat capacity or instrument calibration factor. The working limits for the instrument calibration shall be determined and defined in terms of the corrected temperature rise. All subsequent measurements shall be kept within these limits.

10.9.3 A convenient way to check a previously calibrated instrument is to use benzoic acid as an unknown. The mean value for the heat of combustion from duplicate runs using 0.7 g and 1.3 g sample masses, respectively, should be within 56 J/g or 24 Btu / lb of the accepted heat of combustion value.

10.9.4 For any given instrument, examination of the applicable range of the instrument calibration should be carried out when the instrument is new, moved to a different location or subject to major repair.

11. Calibration Verification

11.1 The calorimeter calibration shall be checked on a regular basis. Renewed determination of the heat capacity is required whenever significant alterations have been made to the instrument or to the test conditions. The optimum frequency for checking the heat capacity or instrument calibration will depend on the stability of the measurement system and the risk involved when the system departs from statistical control. Since all data obtained during the period last-known-in-control to first-known-out-of-control are suspect, such intervals may need to be minimized.

11.1.1 There are several empirical approaches to deciding on how frequently the instrument calibration should be checked. The experience of the laboratory may indicate the expected frequency of occurrence of trouble, in which case reference sample measurements, at least three in number, should be equally spaced within such an interval. Another approach is the "length of run" concept. In this, recognizable breaks in the production (of data) process are identified which could cause significant changes in precision or bias. Such breaks could include change of work shift; rest periods; change, modification, or adjustment of apparatus; use of new calibration standards; significantly long down-times; use of a new lot of reagents. At least three reference samples should be measured during any of these periods when the periods are considered to be potentially significant.

11.1.2 Periodic checks of the instrument calibration are a risk-reducing procedure. However, if it involves more than ten percent of a laboratory's measurement effort, either the quality

control process may need improvement or too much effort is being exerted in this direction. If less than five percent of effort is devoted to such measurements, the laboratory may be taking too high a risk of producing unacceptable data, or may not even know the quality of the data it is producing. The above statements are made with a laboratory making a significant number of high-quality routine measurements in mind. If a laboratory's program involves occasional or one-of-a-kind measurements, the amount of quality assurance effort required, including the number of measurements of reference materials to be made may be significantly more than that indicated above.

11.1.3 Two complementary procedures are offered for calorimeter calibration verification: Control Chart Method and Rolling Average Method.

11.2 Control Chart Method for Calibration Verification:

11.2.1 A control chart is a graphical way to interpret test data. In its simplest form, a selected reference sample is measured periodically and the results are plotted sequentially (or time-ordered) on a graph. Limits for acceptable values are defined and the measurement system is assumed to be in control (variability is stable and due to chance alone) as long as the results stay within these limits. The residence of the values within expected limits is accepted as evidence that the precision of measurement remains in control. The monitored precision of measurement and the accuracy of measurement of the reference sample may be transferred, by inference, to all other appropriate measurements made by the system while it is in a state of control.

11.2.2 A control chart can be realized by sequentially plotting individual measurement values. The central line is the most probable value for (that is, the grand average) of all the measurements or the accepted measurement value. The limits LWL to UWL (lower and upper warning limits) define the area in which 95 percent of the plotted points are expected to lie. The limits LCL to UCL (lower and upper control limits) define the area in which almost all (99.7%) of the plotted points are expected to lie when the system is in a state of statistical control. It should be clear that when more than 5 percent of the points (one in twenty) lie outside of the warning limits or when values fall outside of the control limits the system is behaving unexpectedly and corrective actions, and even rejection of data, may be required.

11.2.3 Results are expected to scatter with a normal distribution within the limits. Systematic trends or patterns in the data plots may be early warning of incipient problems and are cause for concern; hence techniques to identify such should be practiced.

11.2.4 Control charts, including the factors for calculating control limits are discussed more thoroughly elsewhere (see Guide E882 and **(1)**⁶). The central line is either the known value for the test sample (for example, certified value), or the mean of 10 sets of independent measurements. Control limits are then calculated according to the following relationships.

$$\text{UCL} \qquad \text{Mean or accepted value} + 3 * \sigma / \sqrt{N}$$

⁶ The boldface numbers in parentheses refer to a list of references at the end of this standard.

UWL	Mean or accepted value + 2 * sigma / sqrt(N)
Central Line	Mean of the 10 most recent measurements or the accepted value.
X(bar)	
LWL	Mean or accepted value – 2 * sigma / sqrt(N)
LCL	Mean or accepted value – 3 * sigma / sqrt(N)

For the above limits, N represents the number of repetitive measurements of the reference sample, the mean of which is plotted on an Xbar chart. For an X chart (single measurement of the reference sample) N = 1. The standard deviation of the measurement process is sigma. Sigma is taken as 0.10% of the mean of the ten most recent measurements or 0.10% the accepted value if tests are being performed using a reference material, for example benzoic acid, run as an unknown. **Table 2** illustrates important selected control limits for calorimeter operation when benzoic acid is used as a test sample.

11.3 Rolling Average Method:

11.3.1 The mean value of the ten most recent calorimeter calibration or heat capacity measurements is used to support the calibration of the calorimeter system. A single new value, incorporated into the average of the ten most recent measurements, discarding the oldest measurement in the existing series of ten measurements first, must meet the precision requirements outlined in **10.8.2**.

11.4 Recommended Test Substances:

11.4.1 By international agreement in the 1920's, benzoic acid was selected as the chemical standard to be used in calibrating bomb calorimeters. Today, it remains as the sole chemical primary standard for this type of calibration.

11.4.1.1 In general, the calibration of an analysis instrument consists of the evaluation of its response function in terms of the composition of the analyte. The instrument responds to some property of the analyte, the value of which needs to be quantified by use of known substances. It is tacitly assumed that the instrument will respond analogously to the standard and test samples. With this in mind, the confidence in the measurement process is influenced by the uncertainty in composition of known samples and the soundness of the analogy.

11.4.1.2 It is desirable to perform check experiments in order to demonstrate confidence in the ability to make measurements on unknowns that are not only acceptably precise but also acceptably accurate. This is especially true in instances where conditions in the calibration and combustion tests differ appreciably. For example, large differences in the rates of combustion between the calibrant and the unknown or significant differences in combustion chemistries may give rise to systematic errors that are difficult to detect. The use of test substances in such check experiments can help demonstrate that the techniques and procedures used in determining heats of combustion of unknown materials are reasonably free of persistent errors.

11.4.2 For work with solid samples, the following test substances are recommended.

Substance	-Delta u _B / Jg ⁻¹
Acetanilide CAS 103-84-4 CH ₃ C ₆ H ₄ NHCOCH ₃ MWT 135.17 Density 1.22 g/cc	31279 (2)
Tris (hydroxymethyl) aminomethane CAS 77-86-1 (HOCH ₂) ₃ CN ₂ H MWT 121.14 Density = 1.35 g/cc	20058 (3)

^AMass against stainless steel weights (8 g/cc) in air (0.0012 g/cc).

11.5 Use of Laboratory Control Materials:

11.5.1 A laboratory control material (LCM) is similar to a certified reference material in that it is a homogeneous matrix that offers key characteristics similar to the samples being analyzed. A true LCM is one that is prepared and stored in a stable condition strictly for use in-house by a single laboratory. Alternately, the material may be prepared by a central laboratory and distributed to others (so-called regional or program control materials). Unlike CRMs, the heat of combustion of LCMs are not certified but are based upon a statistically valid number of replicate analyses by one or several laboratories. In practice, this material can be used to assess the performance of a single laboratory, as well as to determine the degree of comparability among different laboratories.

11.5.2 A significant amount of work is involved with the production and maintenance of any LCM. For example, materials related issues such as stability, homogenization techniques and proper conditions for storage must be addressed. For smaller laboratories, the time and effort involved supporting the use of true LCMs may not be justified. In such cases, the use of CRMs is preferred.

11.5.3 Routine analysis of CRMs or LCMs represent an important aspect of a performance-based QA philosophy. At least one CRM or LCM must be analyzed along with each batch of 20 or fewer samples (that is, QA samples should comprise a minimum of 5% of each set of samples). For CRMs, the certified heat of combustion value will be known to the analyst(s) and will be used to provide an immediate check on performance before proceeding with a subsequent sample batch. Performance criteria for both precision and accuracy must be established for the analysis of CRMs or LCMs using a given instrumental technique. If the laboratory fails to meet either the precision or accuracy control limit criteria for a given analysis of the CRM or LCM, the data for the entire batch of samples is suspect. Potential operating deficiencies must be checked / corrected and the CRM or LCM may have to be reanalyzed to confirm the results. If the values are still outside the control limits in the repeat analysis, the laboratory is required to find and eliminate the source(s) of the problem and repeat the analysis of that batch of samples until control limits are met, before final data are reported.

TABLE 2 Calorimeter Control Limits When Benzoic Acid is Used as a Test Sample

NOTE—Accepted heat of combustion taken as 26454 J/g
 Process sigma is 0.10% RSD
 Control limits based on 99% confidence (3 sigma) values
 Values are in J/g except as noted.

Number of Observations in a Group	UCL for the range (High-Low) within the Group	UCL for the RSD within the Group	Maximum Permissible Deviation of the Group Mean from the Accepted Value or Grand Mean
1	79.4
2	97.5	0.2606	56.1
3	115.3	0.2276	45.8
4	124.3	0.2088	39.7
5	130.1	0.1964	35.5
6	134.3	0.1874	32.4
7	137.6	0.1806	30.0
8	140.4	0.1751	28.1
9	142.7	0.1707	26.5
10	144.7	0.1669	25.1
15	151.8	0.1554	20.5
20	156.7	0.1470	17.7
25	160.2	0.1420	15.9

Calorimeter Heat Capacity X Chart

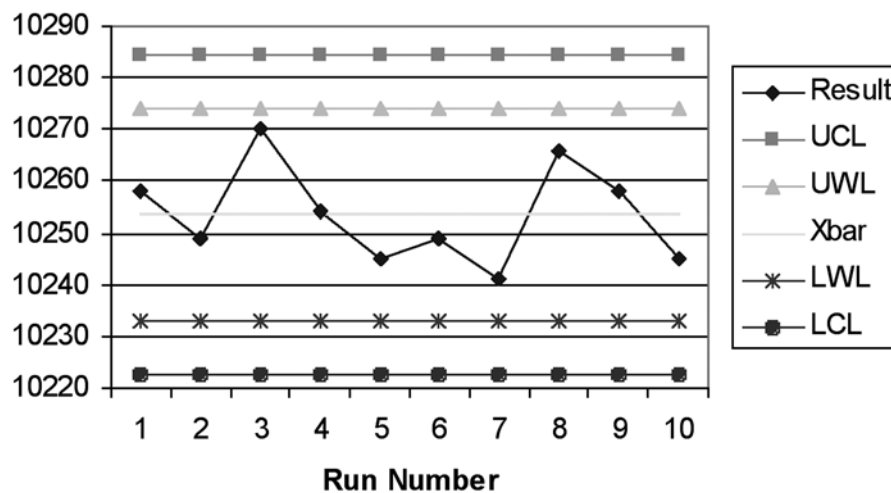


FIG. 1 Example of X Chart for Calibration Runs

12. Procedure for Coal and Coke Samples

12.1 Weigh 0.8 to 1.2 g of sample into a sample holder. Record the weight to the nearest 0.0001 g (see 12.6.3).

12.2 Follow the procedures as described in 10.2-10.5 for determination of heat capacity. For the calorific value of coke, it is necessary to use 3-MPa (30-atm) pressure for both standardization and analysis. The starting temperature for determinations shall be within ±0.5°C of that used in the determination of the heat capacity.

12.2.1 For coke, place a clean combustion capsule in the center of a quartz disk and press the capsule to make an impression in the disk. Cut slits from the outside edge of the disk to the impression. Insert the quartz disk in the combustion capsule so that the slit portion will cover the sides of the capsules.

12.3 Carry out a moisture determination in accordance with Test Method D3173 or Test Methods D5142 on a separate

portion of the analysis sample preferably on the same day but not more than 24 h apart from the calorific value determination so that reliable corrections to other bases can be made.

12.4 Conduct the sulfur analysis in accordance with Test Methods D3177 or D4239. From the weight % sulfur, calculate the sulfur corrections (see X1.2):

$$e3 = 55.2 \text{ J/g} \times S \times m \text{ (13.18 cal/g} \times S \times m) \quad (8)$$

where:

$e3$ = a correction for the difference between the heat of formation of H_2SO_4 from SO_2 with respect to the formation of HNO_3 , J;

S = wt % sulfur in the sample; and

m = mass of sample from 12.1, g.

12.4.1 When titration method is used (see 10.6.1.1), the sulfur correction is

$$e3 = 55.18 \text{ J/g} \times S \times m \text{ or (13.18 cal/g} \times S \times m) \quad (9)$$

Benzoic Acid Check Sample X Chart

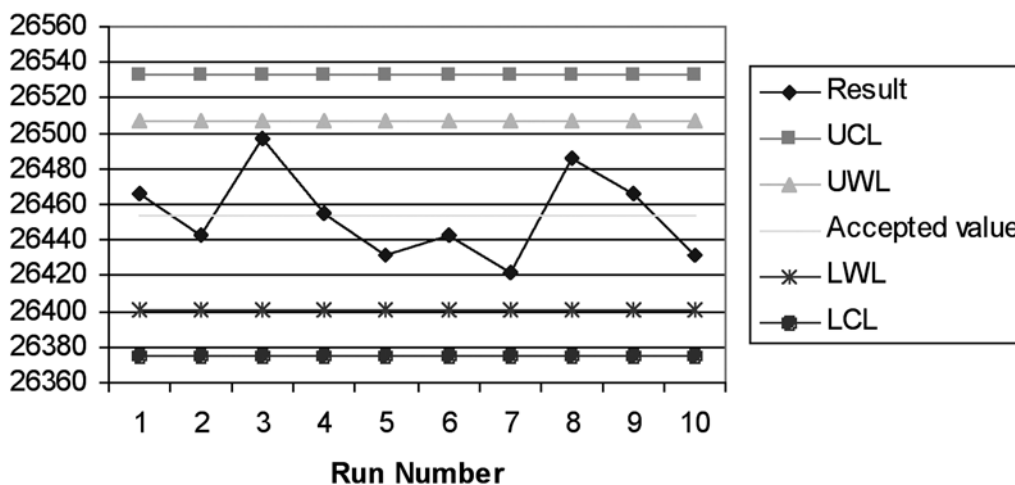


FIG. 2 Example of X Chart for Check Sample Runs

12.4.2 When the calculated nitric acid method is used (see 10.6.1.2), the sulfur correction is

$$e3 = 94.51 \text{ J/g} \times S \times m \text{ or } (22.57 \text{ cal/g} \times S \times m) \quad (10)$$

12.5 For eight mesh samples, analyze coals susceptible to oxidation within 24 h of preparation.

12.6 Coal or coke that do not burn completely can be treated as follows:

12.6.1 For coke, use a crucible liner of the type recommended in 6.11.

12.6.2 Use a combustion aid such as benzoic acid, ethylene glycol, mineral oil or a gelatin capsule. A minimum of 0.4 g of combustion aid shall be used. Record the weight to the nearest 0.0001 g. Calculate the correction for use of a combustion aid using the following:

$$e4 = Ha \times ma \quad (11)$$

where:

$e4$ = correction for use of a combustion aid,
 Ha = heat of combustion of the combustion aid J/g (cal/g),
 and

ma = mass of combustion aid, g.

$$[(EE \times t) - e1 - e2 - e3 - e4] / m$$

12.6.3 Vary the mass of the sample to obtain good ignition and so that the total heat generated is the same as the heat generated during calibration.

13. Calculation

13.1 *Gross Calorific Value*—Calculate the gross calorific value $Q_{vad}(\text{gross})$ using the following equation:

$$Q_{vad}(\text{gross}) = [(tE_e) - e1 - e2 - e3 - e4] / m \quad (12)$$

where:

$Q_{vad}(\text{gross})$ = gross calorific value at constant volume as determined, J/g (cal/g);
 E_e = the heat capacity of the calorimeter, J/°C (cal/°C);

t = corrected temperature rise according to 10.7, °C;

$e1$ = acid correction according to 10.6.1, J;

$e2$ = fuse correction according to 10.6.2, J;

$e3$ = sulfur correction determined according to 12.4, J;

$e4$ = combustion aid correction determined according to 12.6.2, J; and

m = mass of the sample, g.

13.1.1 See X1.2.3 for an example calculation.

13.2 *Net Calorific Value at Constant Pressure*:

13.2.1 Several steps are required in order to report an as-received net heat of combustion, at constant pressure, derived from an as-determined gross heat of combustion at constant volume. The first step involves calculating a gross heat of combustion at constant pressure from the calorimetrically determined gross heat of combustion in the bomb at constant volume.

13.2.2 No work is performed in constant-volume bomb calorimetry, so the heat measured equals the change in internal energy of the system. When fuel is burned at constant pressure, there is a change in the volume of the system. A small change in energy accompanies this change in volume. When fuel is burned at constant pressure and the water formed condensed to the liquid state, there is a contraction in the volume of the system. This contraction is equal to the volume of oxygen required to burn the hydrogen. Work is done on the system by the atmosphere in filling this void in order to maintain a constant pressure. When carbon in the fuel reacts with oxygen, an equal volume of carbon dioxide results and no change in volume occurs. The oxygen and nitrogen in the fuel both give rise to an increase in volume. The energy associated with this change in the volume of the gaseous phase for the combustion reaction may be expressed as follows.

$$Q_{v-p} = 0.01 * RT * (H_{ad} / (2 * 2.016) - O_{ad} / 31.9988 - N_{ad} / 28.0134) \quad (13)$$

R is the universal gas constant [8.3143 J/(mol *K)] and T is the

standard thermochemical reference temperature (298.15 K).

13.2.2.1 H_{ad} , O_{ad} and N_{ad} are as-determined hydrogen, oxygen and nitrogen, respectively, %, in the analysis sample. The hydrogen and oxygen contributed by the sample moisture are not included in H_{ad} and O_{ad} , respectively.

13.2.2.2 The following formulas may be used to convert hydrogen and oxygen values that include the hydrogen and oxygen in the moisture associated with the analysis sample to values excluding the moisture.

$$H_{ad} = H_{ad,m} - 0.1119 * M_{ad} \quad (14)$$

$$O_{ad} = O_{ad,m} - 0.8881 * M_{ad} \quad (15)$$

13.2.3 The next steps involve calculating the energy associated with the heat of vaporization of water that originates from the hydrogen content of the sample [Qh], the moisture content of the analysis sample [Qmad] as well as the as-received moisture value [Qmar].

$$Qh = 0.01 * H_{vap} * (H_{ad} / 2.016) \quad (16)$$

H_{vap} is the constant pressure heat of vaporization of water at 25 C (43985 J/mol).

$$Q_{mad} = 0.01 * H_{vap} * (M_{ad} / 18.0154) \quad (17)$$

$$Q_{mar} = 0.01 * H_{vap} * (M_{ar} / 18.0154) \quad (18)$$

M_{ad} and M_{ar} are values for moisture as-determined and as-received, respectively in weight %.

13.2.4 The as-determined net heat of combustion at constant pressure is equal to calorimetrically determined heat of combustion with the addition of the small constant volume to constant pressure correction, less the energy associated with the latent heat of vaporization of water originating from the fuel hydrogen and the sample moisture.

$$Q_{pad(net)} = Q_{vad(gross)} + Q_{v-p} - Qh - Q_{mad} \quad (19)$$

13.2.5 The dry net heat of combustion at constant pressure is given by the following relationship.

$$Q_{pd(net)} = (Q_{vad(gross)} + Q_{v-p} - Qh) * (100 / (100 - M_{ad})) \quad (20)$$

13.2.6 The as-received net heat of combustion at constant pressure is given by the following relationship.

$$Q_{par(net)} = (Q_{vad(gross)} + Q_{v-p} - Qh) * (100 - M_{ar}) / (100 - M_{ad}) - Q_{mar} \quad (21)$$

13.2.7 For reference purposes, the dry and as-received gross heat of combustion values at constant volume are provided by the following well-known relationships described in Practice D3180.

$$Q_{vd(gross)} = Q_{vad(gross)} * (100 / (100 - M_{ad})) \quad (22)$$

$$Q_{var(gross)} = Q_{vad(gross)} * (100 - M_{ar}) / (100 - M_{ad}) \quad (23)$$

Example:

Q _{vd(gross)}	30000 J/g
M _{ad}	2.00%
M _{ar}	8.00%
H(ad)	4.00%
O(ad)	13.00%
N(ad)	1.00%
Q _{v-p}	13.6 J/g
Q _h	872.7 J/g
Q _{mad}	48.8 J/g

Q _{mar}	195.3 J/g
Q _{var}	28163.3 J/g
Q _{pad(net)}	29092.1 J/g
Q _{pd(net)}	29735.6 J/g
Q _{par(net)}	27161.5 J/g

14. Report

14.1 Report the calorific value as Q_{vad} (gross) along with the moisture of the sample as determined M_{ad} from 12.3.

14.2 The results of the calorific value can be reported in any of a number of bases differing in the manner the moisture is treated. Procedures for converting the value obtained on an analysis sample to other bases are described in Practice D3180.

15. Precision and Bias^{3,5}

15.1 Precision

15.1.1 Manual Adiabatic Calorimeters

15.1.1.1 250 μm (No. 60) Samples:

(1) *Repeatability Limit (r)*—The value below which the absolute difference between two test results calculated to a dry basis (Practice D3180) of separate and consecutive test determinations, carried out on the same sample of 250 μm (No. 60) coal and coke in the same laboratory by the same operator using the same apparatus on samples taken at random from a single quantity of homogeneous material, may be expected to occur with a probability of approximately 95 %. The repeatability limit for this test method is 115 J/g (50 Btu/lb).

(2) *Reproducibility Limit (R)*—The value below which the absolute difference between two test results calculated to a dry basis (Practice D3180) carried out in different laboratories using samples of 250 μm (No. 60) coal and coke taken at random from a single quantity of material that is as homogeneous as possible, may be expected to occur with a probability of approximately 95 %. The reproducibility limit for this test is 250 J/g (100 Btu/lb).

15.1.1.2 2.36 mm (No. 8) Samples:⁷

(1) *Repeatability Limit (r)*—The value below which the absolute difference between two test results calculated to a dry basis (Practice D3180) of separate and consecutive test determinations, carried out on the same sample, using the same riffle, determined on a single test specimen of two separate 2.36 mm (No. 8) test units of coal reduced entirely to 250 μm (No. 60) and prepared from the same bulk sample coal in the same laboratory by the same operator using the same apparatus on samples taken at random from a single quantity of homogeneous material, may be expected to occur with a probability of approximately 95 %.

(2) *Reproducibility Limit (R)*—The value below which the absolute difference between two test results calculated to a dry basis (Practice D3180) carried out in different laboratories using samples of 2.36 mm (No. 8) coal reduced entirely to 250 μm (No. 60) taken at random from a single quantity of material

⁷ An interlaboratory study, designed consistent with Practice E691, was conducted in 1989. Eight laboratories participated in this study. Supporting data are available from ASTM Headquarters. Request Report RR:D05-1015.

TABLE 3 Ranges and Limits of Repeatability for the Gross Calorific Value of 2.36 mm (No.8) Coal with Manual Adiabatic Calorimeters

Coal	Range	Repeatability Limit (<i>r</i>)
Bituminous	29 535 to 33 720 J/g (12 700 to 14 500 Btu/lb)	160 J/g (69 Btu/lb)
Subbituminous-Lignite	20 442 to 29 651 J/g (8790 to 12 750 Btu/lb)	140 J/g (59 Btu/lb)

that is as homogeneous as possible, may be expected to occur with a probability of approximately 95 %.

TABLE 4 Ranges and Limits of Reproducibility for the Gross Calorific Value of 2.36 mm (No.8) Coal with Manual Adiabatic Calorimeters

Coal	Range	Reproducibility Limit (<i>R</i>)
Bituminous	29 535 to 33 720 J/g (12 700 to 14 500 Btu/lb)	249 J/g (107 Btu/lb)
Subbituminous-Lignite	20 442 to 29 651 J/g (8790 to 12 750 Btu/lb)	326 J/g (140 Btu/lb)

15.1.2 Automated Calorimeters

15.1.2.1 Microprocessor Controlled Calorimeters:⁸

(1) *Precision*—The precision of this method for the determination of caloric value in the analysis sample of coal and coke is shown in **Tables 5 and 6**. The precision characterized by repeatability (S_p , *r*) and reproducibility (S_R , *R*) is described in **Table A2.1** in **Annex A2**.

(1) *Repeatability Limit (r)*—250 μm (No. 60) Samples—the value below which the absolute difference between two test results calculated to a dry basis (Practice **D3180**) of separate and consecutive test determinations, carried out on the same sample of 250 μm (No. 60) coal and coke in the same laboratory by the same operator using the same apparatus with the same heat capacity on samples taken at random from a

⁸ An interlaboratory study, designed consistent with Practice E691, was conducted in 1995. Twelve labs participated in this study. Supporting data are available from ASTM Headquarters. Request Report RR:D05-1020.

TABLE 5 Ranges and Limits of Repeatability for the Gross Calorific Value of 250 μm (No. 60) Coal with Microprocessor Controlled Calorimeters

Coal	Range	Repeatability Limit (<i>r</i>)
Bituminous	26 280 to 34 190 J/g (11 300 to 14 700 Btu/lb)	149 J/g (64 Btu/lb)
Subbituminous-Lignite	21 860 to 27 680 J/g (9400 to 11 900 Btu/lb)	193 J/g (83 Btu/lb)

TABLE 6 Ranges and Limits of Reproducibility for the Gross Calorific Value of 250 μm (No. 60) Coal with Microprocessor Controlled Calorimeters

Coal	Range	Reproducibility Limit (<i>R</i>)
Bituminous	26 280 to 34 190 J/g (11 300 to 14 700 Btu/lb)	256 J/g (110 Btu/lb)
Subbituminous-Lignite	21 860 to 27 680 J/g (9400 to 11 900 Btu/lb)	381 J/g (164 Btu/lb)

single quantity of homogeneous material, may be expected to occur with a probability of approximately 95 %.

(2) *Reproducibility Limit (R)*—250 μm (No. 60) Samples—the value below which the absolute difference between two test results calculated to a dry basis (Practice **D3180**) carried out in different laboratories using samples of 250 μm (No. 60) coal and coke taken at random from a single quantity of material that is as homogeneous as possible, may be expected to occur with a probability of approximately 95 %.

NOTE 2—Calorific values have not been determined for anthracite coals.

NOTE 3—Precision statements have not been determined for No. 8 sieve size coal.

15.2 *Bias*—Bias in the determination of the gross calorific value is eliminated provided samples are treated identically to the benzoic acid used in the determination of the calorimeter heat capacity.

16. Keywords

16.1 adiabatic calorimeter; bomb calorimeters; calorific value; calorimeter; coal; coke; isoperibol bomb calorimeter

ANNEXES

(Mandatory Information)

A1. THERMOMETRIC CORRECTIONS

A1.1 *Thermometer Corrections*—The following corrections shall be made:

A1.1.1 *Calibration Correction*, shall be made in accordance with the calibration certificate furnished by the calibration authority.

A1.1.2 *Radiation Corrections*—Radiation corrections are required to calculate heat loss or gain to the isoperibol water jacket. They are based on the Dickinson formula,(4) the

Regnault-Pfaundler formula,(5) or the U.S. Bureau of Mines method.(6) The same method of determining the radiation correction shall be used consistently in the determination of heat capacity and sample measurements.

A1.1.2.1 *Dickinson Formula*:

$$C_r = -r1 \times (b - a) - r2 \times (c - b) \quad (\text{A1.1})$$

where:

- C_r = radiation correction;
 $r1$ = rate of rise in temperature per minute in the preliminary period;
 $r2$ = rate of rise of temperature per minute in the final period (if temperature is falling, $r2$ is negative);
 ta = firing temperature;
 tc = final temperature, being the first temperature after which the rate of change is constant;
 a = time at temperature ta , min;
 b = time at temperature $ta + 0.60(tc - ta)$, min; and
 c = time at temperature tc , min.

A1.1.2.2 Regnault-Pfaundler Formula:

$$C_r = nr1 + kS \quad (\text{A1.2})$$

where:

- C_r = radiation correction,
 n = number of minutes in the combustion period,

$$k = (r1 - r2) / (t'' - t'), \quad (\text{A1.3})$$

$$S = tn - 1 + (1/2)(ti + tf)nt' \quad (\text{A1.4})$$

- t' = average temperature during the preliminary period,
 t'' = average temperature during the final period,
 $r1, r2$ see [A1.1.2.1](#),

$t1, t2, \dots, tm$ = successive temperature recorded during the combustion period, at 1-min intervals, and

$$tm - 1 = \text{sum of } t1, t2, t3 \dots tm - 1 \quad (\text{A1.5})$$

A1.1.2.3 Bureau of Mines Method—A table of radiation corrections can be established so that only the initial and final readings are required to determine the calorific value of a fuel. This can be done by carrying out a series of tests using the procedure described in Section 10, using the following conditions. Regulate the amount of sample burned so that a series of determinations is made in which different temperature rises are obtained. For all determinations, keep the water jacket temperature constant, fire the bomb at the same initial temperature, and have the same time, $c - a$, elapse (± 2 s) between the initial and final readings. Determine the radiation corrections for each of the series of temperature rises using the Dickinson method (see [A1.1.2.1](#)), or the Regnault-Pfaundler method (see [A1.1.2.2](#)). These corrections are constant for a given temperature rise. From the series of readings, a table or graph is plotted to show radiation correction versus temperature rise. Once the table or graph is established, the radiation corrections can be obtained from it until there is a major change in the equipment.

A1.1.3 Emergent Stem Correction

The calculation of emergent stem correction depends upon the way the thermometer was calibrated and how it is used. Two conditions are possible.

A1.1.3.1 Thermometers Calibrated in Total Immersion and Used in Partial Immersion

This emergent stem correction is made as follows:

$$Ce = K(tf - ti)(tf + ti - L - T) \quad (\text{A1.6})$$

where:

- Ce = emergent stem correction,
 K = differential coefficient of thermal expansion for the thermometric liquid, (See [Note A1.1](#).)
 L = scale reading to which the thermometer was immersed,
 T = mean temperature of emergent stem,
 ti = initial temperature reading, and
 tf = final temperature reading.

NOTE A1.1—Typically 0.00076 for thermometers calibrated in °C and filled with a low hazard thermometric liquid.

Example:

A thermometer was immersed to 16°C; its initial reading, ti , was 24.127°C; its final reading, tf , was 27.876; the mean temperature of the emergent stem, T , was 26°C.

$$Ce = 0.00076 \times (27.9 - 24.1) \times (27.9 + 24.1 - 16 - 26) = 0.029 \quad (\text{A1.7})$$

A1.1.3.2 Thermometers Calibrated and Used in Partial Immersion, But at a Different Temperature Than the Calibrated Temperature:

$$Ce = K(tf - ti)(tc - to) \quad (\text{A1.8})$$

where:

- Ce = emergent stem correction,
 K = differential coefficient of thermal expansion for the thermometric liquid, (See [Note A1.2](#).)
 ti = initial temperature reading,
 tf = final temperature reading,
 to = observed stem temperature, and
 tc = stem temperature at which the thermometer was calibrated.

NOTE A1.2—Typically 0.00076 for thermometers calibrated in °C and filled with a low hazard thermometric liquid.

Example:

A thermometer has an initial reading, ti , 27°C; a final reading, tf , 30°C; the observed stem temperature, to , 28°C; and the calibration temperature, tc , 22°C.

$$Ce = 0.00076 \times (30 - 27) \times (28 - 22) = 0.014 \quad (\text{A1.9})$$

A2. PRECISION STATISTICS

A2.1 The precision of this test method, characterized by repeatability (S_r, r) and reproducibility (S_R, R) has been determined for the following materials as listed in [Table A2.1](#).

A2.2 Repeatability Standard Deviation (S_r)—The standard deviation of test results obtained under repeatability conditions.

A2.3 Reproducibility Standard Deviation (S_R)—The standard deviation of test results obtained under reproducibility conditions.

TABLE A2.1 Repeatability (S_r , r) and Reproducibility (S_R , R) Parameters Used for Calculation of Precision Statement

Material	Average	S_r	S_R	r	R
91-2 lvb	14473.32	19.95	44.67	55.81	124.98
91-1 hvAb	14719.75	25.68	40.04	71.86	112.02
91-5 hvAb	12927.36	24.09	35.78	67.41	100.11
89-4 hvCb	11976.68	28.72	29.74	80.37	83.20
91-4 hvCb	11303.64	14.09	47.50	39.41	132.91
90-1 subB	9416.21	20.10	69.92	56.25	195.65
89-7 subA	11979.54	37.51	47.70	104.94	133.46
91-6 subA	11395.46	27.26	59.43	76.26	166.28
89-6 subC	9981.04	27.50	58.44	76.94	163.51
Lignite	9659.36	34.26	57.67	95.85	161.35

APPENDIX


(Nonmandatory Information)

X1. THERMOCHEMICAL CORRECTIONS

X1.1 Energy of Formation of Nitric Acid (HNO_3):

X1.1.1 A correction, $e1$, (10.6.1) is applied for the formation of nitric acid.

X1.1.2 (1) HNO_3 is formed in the calorimeter by the following reaction:



X1.1.3 (2) the energy of formation of HNO_3 in approximately 500 mol of water under bomb conditions is minus 59.0 kJ/mol (14.09 Kcal/mole).(7)

X1.1.4 Normal convention assigns a negative value for a heat of formation that is exothermic. By definition, heat released from combustion processes are expressed as positive values. Hence, the negative factors developed for nitric and sulfuric acid corrections are expressed as positive values in the calculations.


X1.1.5 A convenient concentration of Na_2CO_3 is 3.76-g Na_2CO_3/L which gives $e1 = V$ where V is the volume of Na_2CO_3 in millilitres. When H_2SO_4 is produced during the combustion of coal or coke, a part of the correction for H_2SO_4 is present in the $e1$ correction. The remainder is in the $e3$ correction (see X1.2).

X1.2 Energy of Formation of Sulfuric Acid (H_2SO_4)—By definition (see Terminology D121), the gross calorific value is obtained when the product of the combustion of sulfur in the sample is $SO_2(g)$. However, in actual bomb combustion processes, all the sulfur is found as H_2SO_4 in the bomb washings.

X1.2.1 A correction $e3$ is applied for the sulfur that is converted to H_2SO_4 . This correction is based upon the energy of formation of H_2SO_4 in solutions, such as will be present in the bomb at the end of a combustion from SO_2 . This energy is taken as -297.2 kJ/mol.(8)

X1.2.2 When the bomb washings are titrated, a correction of 2×59.7 kJ/mole of sulfur is applied in the $e1$ correction so that the additional correction that is necessary is the difference in the heats of formation for nitric and sulfuric acid and this correction is $-297.2 - (-2 \text{ times } 59.7) = -177.8$ kJ/mol, or -55.45 J/g (13.2 cal/g) of sulfur times the weight of sample in grams times percent sulfur in sample.

X1.2.3 If a 1-g sample is burned, the resulting H_2SO_4 condensed with water formed on the walls of the bomb will have a ratio of about 15 mol of water to 1 mol of H_2SO_4 . For this concentration, the energy of the reaction under the conditions of the bomb process is -303 kJ/mole.



X1.2.4 The values above are based on a sample containing approximately 5 % sulfur and approximately 5 % hydrogen. The assumption is also made that the H_2SO_4 is dissolved entirely in the water condensed during combustion of the sample.(9)

X1.2.5 For different sample weights or sulfur content, or both, the resultant normality of acid formed can be different, and therefore, the normality of titrant must be adjusted accordingly. Basing the calculation upon a sample of comparatively large sulfur content reduces the possible overall errors, because, for small percentages of sulfur, the correction is smaller.

X1.3 Fuse Correction—The energy required to melt a platinum or palladium wire is constant for each experiment if the same amount of platinum or palladium wire is used. As the energy is small, its effect is essentially cancelled out in the relationship between the standardization experiments and the calorific value determinations, and it can be neglected.

X1.4 Reporting Results in Other Units:

X1.4.1 The gross calorific value can be expressed in joules per gram, calories per gram, or British thermal units per pound. The relationships between these units are given in the table below:

1 Btu = 1055.06 J
1 calorie IT = 4.1868 J (10)

1 J/g = 0.430 Btu/lb
1 J/g = 0.239 cal/g
1 cal/g = 1.8 Btu/lb

X1.5 Sample Calculations:

X1.5.1 Heat Capacity:

$$E = [(Hc \times m) + e1 + e2]/t$$

$$Hc = 26\,435 \text{ J/g,}$$

$$m = 1.0047 \text{ g,}$$

$$e1 = 43\text{-J acid correction,}$$

$$e2 = 55\text{-J fuse correction,}$$

$$t = 2.6006^\circ\text{C,}$$

$$E = [(26\,435 \text{ J/g} \times 1.0047 \text{ g}) + 43 \text{ J} + 55 \text{ J}]/2.6006^\circ\text{C, and}$$

$$E = 10\,250.4 \text{ J}^\circ\text{C.}$$

X1.6 Heat of Combustion:

$$Q_{\text{vad}} (\text{gross}) = [(tE) - e1 - e2 - e3 - e4]/m;$$

$$E_e = 10\,250.4 \text{ J}^\circ\text{C;}$$

$$t = 2.417^\circ\text{C;}$$

$$e1 = 77\text{-J acid correction;}$$

$$e2 = 52\text{-J fuse correction;}$$

$$e3 = 58 \times 1.24 \% \times 0.7423 \text{ g, sulfur correction;}$$

$$e4 = 46\,025 \text{ J/g} \times 0.2043 \text{ g, combustion aid correction;}$$

$$m = 0.7423 \text{ g, mass of sample;}$$

$$Q_{\text{vad}} = [(10\,250.4 \text{ J}^\circ\text{C} \times 2.417^\circ\text{C}) - 77 \text{ J} - 52 \text{ J} - 53 \text{ J} - 9403 \text{ J}]/0.7423 \text{ g; and}$$

$$Q_{\text{vad}} = 20\,464 \text{ J/g.}$$

REFERENCES

- (1) ASTM Manual on Presentation of Data and Control Chart Analysis (MNL 7A)
- (2) Johnson, W.H., "The Enthalpies of Combustions and Formation of Acetanilide and Urea," *J.Res.Nat.Bur.Stand.* 1975, 79a, 487.
- (3) Laynez, J., Ringner, B., Sunner, S. J., "On the accuracy of rotating-bomb combustion calorimetry for organic chlorine and bromide compounds," *Chem Thermodynamics* 1970, 2, 603.
- (4) Dickinson, H. C., *Bulletin*, U.S. Bureau of Standards, Vol. 11, 1951, p. 189
- (5) Pfaundler, L., *Annalen der Physik* (Leipzig), ANPYA, Vol. 129, 1966, p. 102.
- (6) Methods of Analyzing & Testing Coal and Coke," U.S. Bureau of Mines *Bulletin* 638, XMBUA, 1967, pp. 16–17.
- (7) Mott, R. A., and Parker, C., "Studies in Bomb Calorimetry IV—Corrections," *Fuel, FUELB*, Vol. 34, 1955, p. 303–316.
- (8) The NBS Tables of Chemical Thermodynamic Properties, Selected Values for Inorganic and C₁ and C₂ Organic Substances in SI Units, *Journal of Phys. Chem. Ref. Data*, 11, Supplement No. 2, 1985, 392 pp.
- (9) Mott, R. A., and Parker, C., "Studies in Bomb Calorimetry IX—Formation of Sulfuric Acid," *Fuel, Fuel B*, Vol. 37, 1958, p. 371.
- (10) Cohen, E. R., and Taylor, B. N., "The 1986 CODATA Recommended Values for the Fundamental Physical Constants," *Journal of Phys. Chem. Ref. Data*, Vol 17, No. 4, 1988, pp. 1795–1803.

SUMMARY OF CHANGES

Committee D05 has identified the location of selected changes to this standard since the last issue (D5865–10) that may impact the use of this standard. (Approved May 1, 2010.)

- (I) 6.6 was revised.

Committee D05 has identified the location of selected changes to this standard since the last issue (D5865–07a) that may impact the use of this standard.

- (I) 13.2.2 was revised.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).